

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG080122\
Data File : FG010251.D
Signal(s) : FID1A.ch
Acq On : 01 Aug 2022 11:33
Operator : YP\AJ
Sample : PB146616BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 02 02:09:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG072822.M
Quant Title :
QLast Update : Thu Jul 28 15:10:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.805	2201256	17.328 ug/ml
Target Compounds			
16) N-HEXATRIACONTANE	20.226	88087	0.764 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG080122\
Data File : FG010251.D
Signal(s) : FID1A.ch
Acq On : 01 Aug 2022 11:33
Operator : YP\AJ
Sample : PB146616BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 02 02:09:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG072822.M
Quant Title :
QLast Update : Thu Jul 28 15:10:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

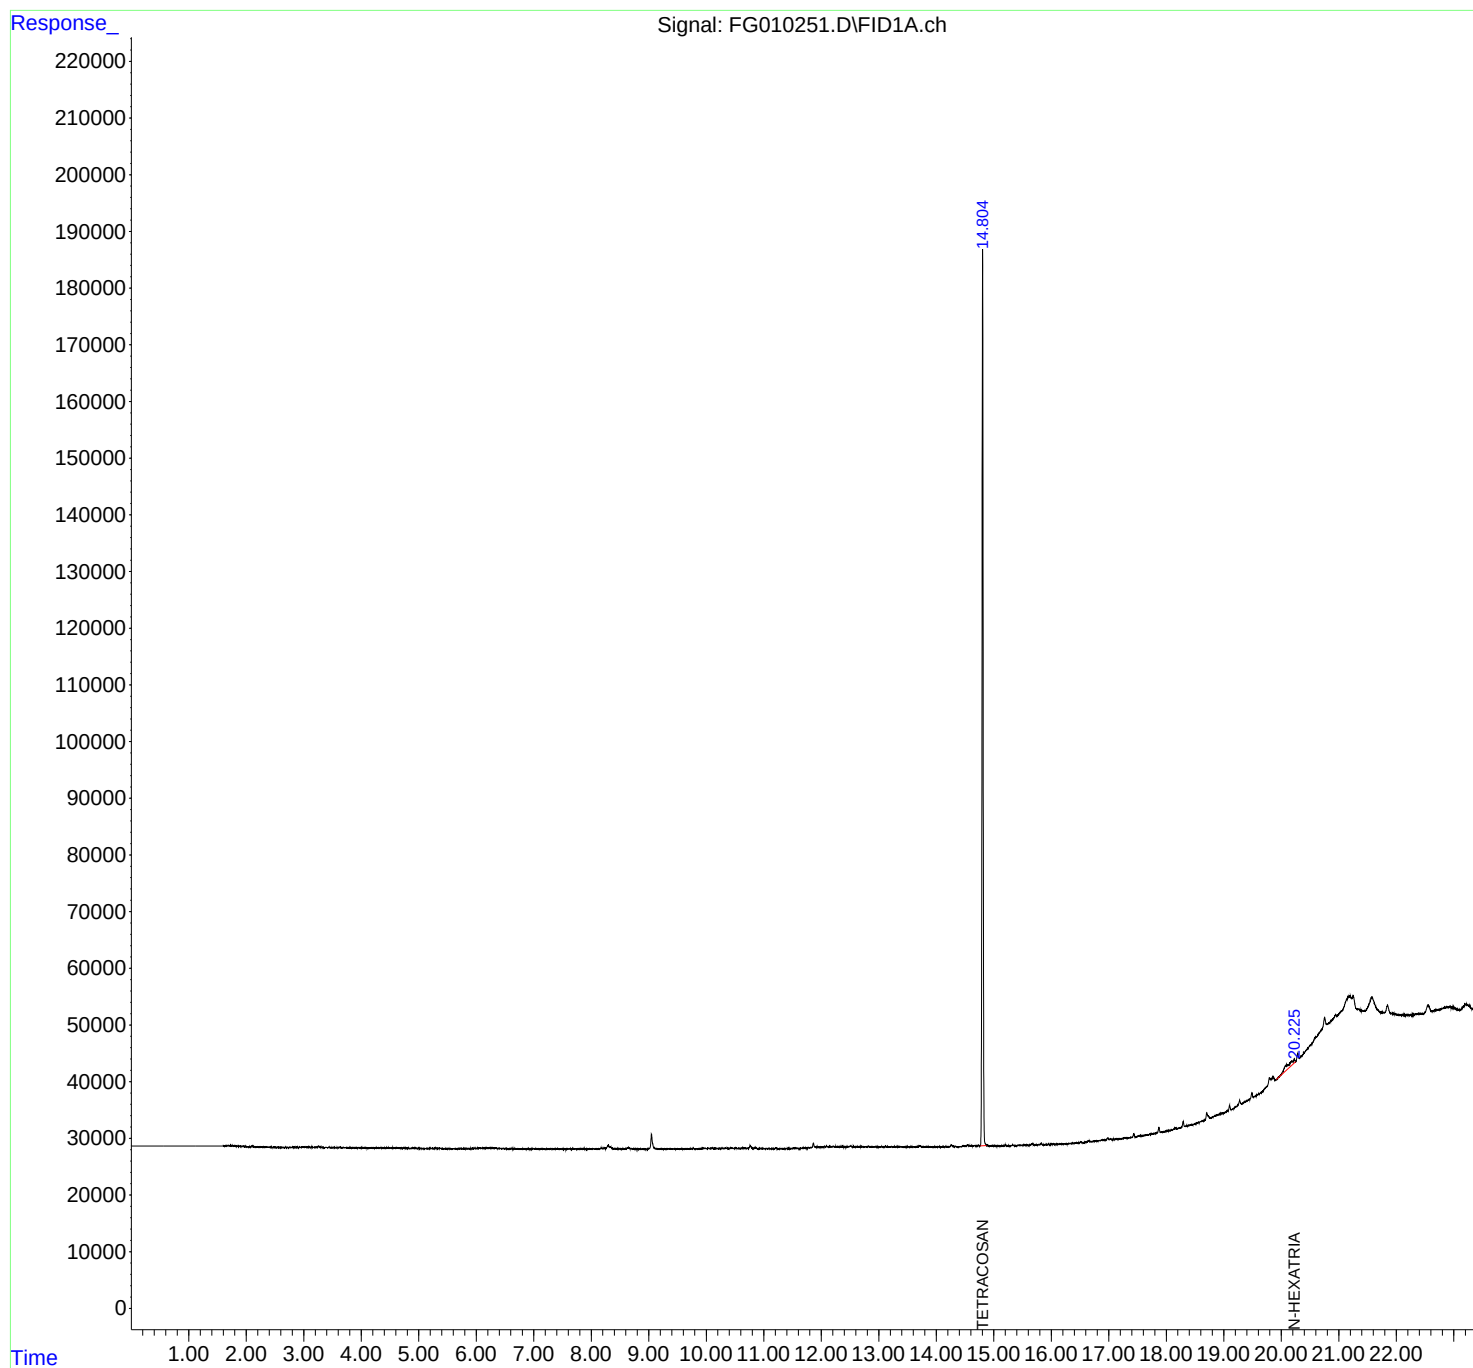


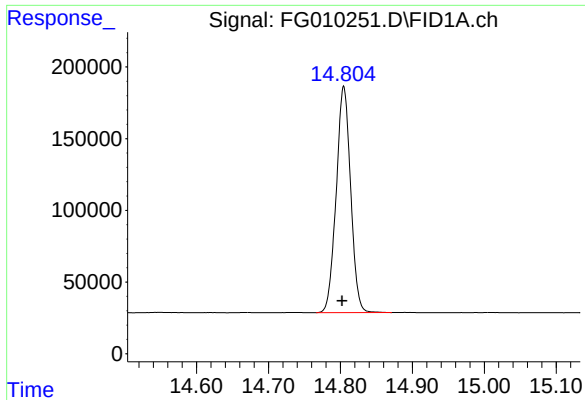

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.805 min
Delta R.T.: 0.002 min
Response: 2201256
Conc: 17.33 ug/ml

Instrument :
FID_G
ClientSampleId :

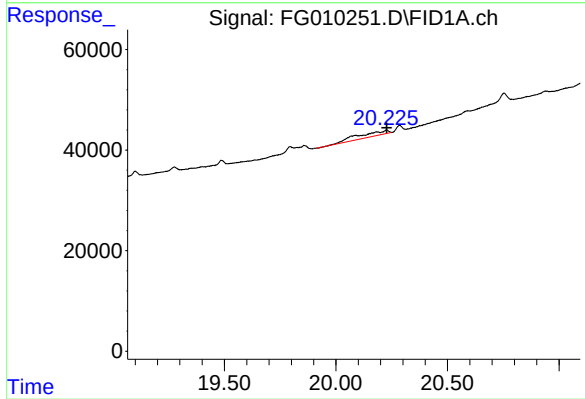

#16 N-HEXATRIACONTANE

R.T.: 20.226 min
Delta R.T.: -0.002 min
Response: 88087
Conc: 0.76 ug/ml