

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG080122\
 Data File : FG010255.D
 Signal(s) : FID1A.ch
 Acq On : 01 Aug 2022 14:02
 Operator : YP\AJ
 Sample : N3965-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 02 02:10:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG072822.M
 Quant Title :
 QLast Update : Thu Jul 28 15:10:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.801	2319982	18.263 ug/ml
Target Compounds			
18) N-TETRACONTANE	21.744	452435	3.856 ug/ml


(f)=RT Delta > 1/2 Window (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG080122\
 Data File : FG010255.D
 Signal(s) : FID1A.ch
 Acq On : 01 Aug 2022 14:02
 Operator : YP\AJ
 Sample : N3965-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 02 02:10:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG072822.M
 Quant Title :
 QLast Update : Thu Jul 28 15:10:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

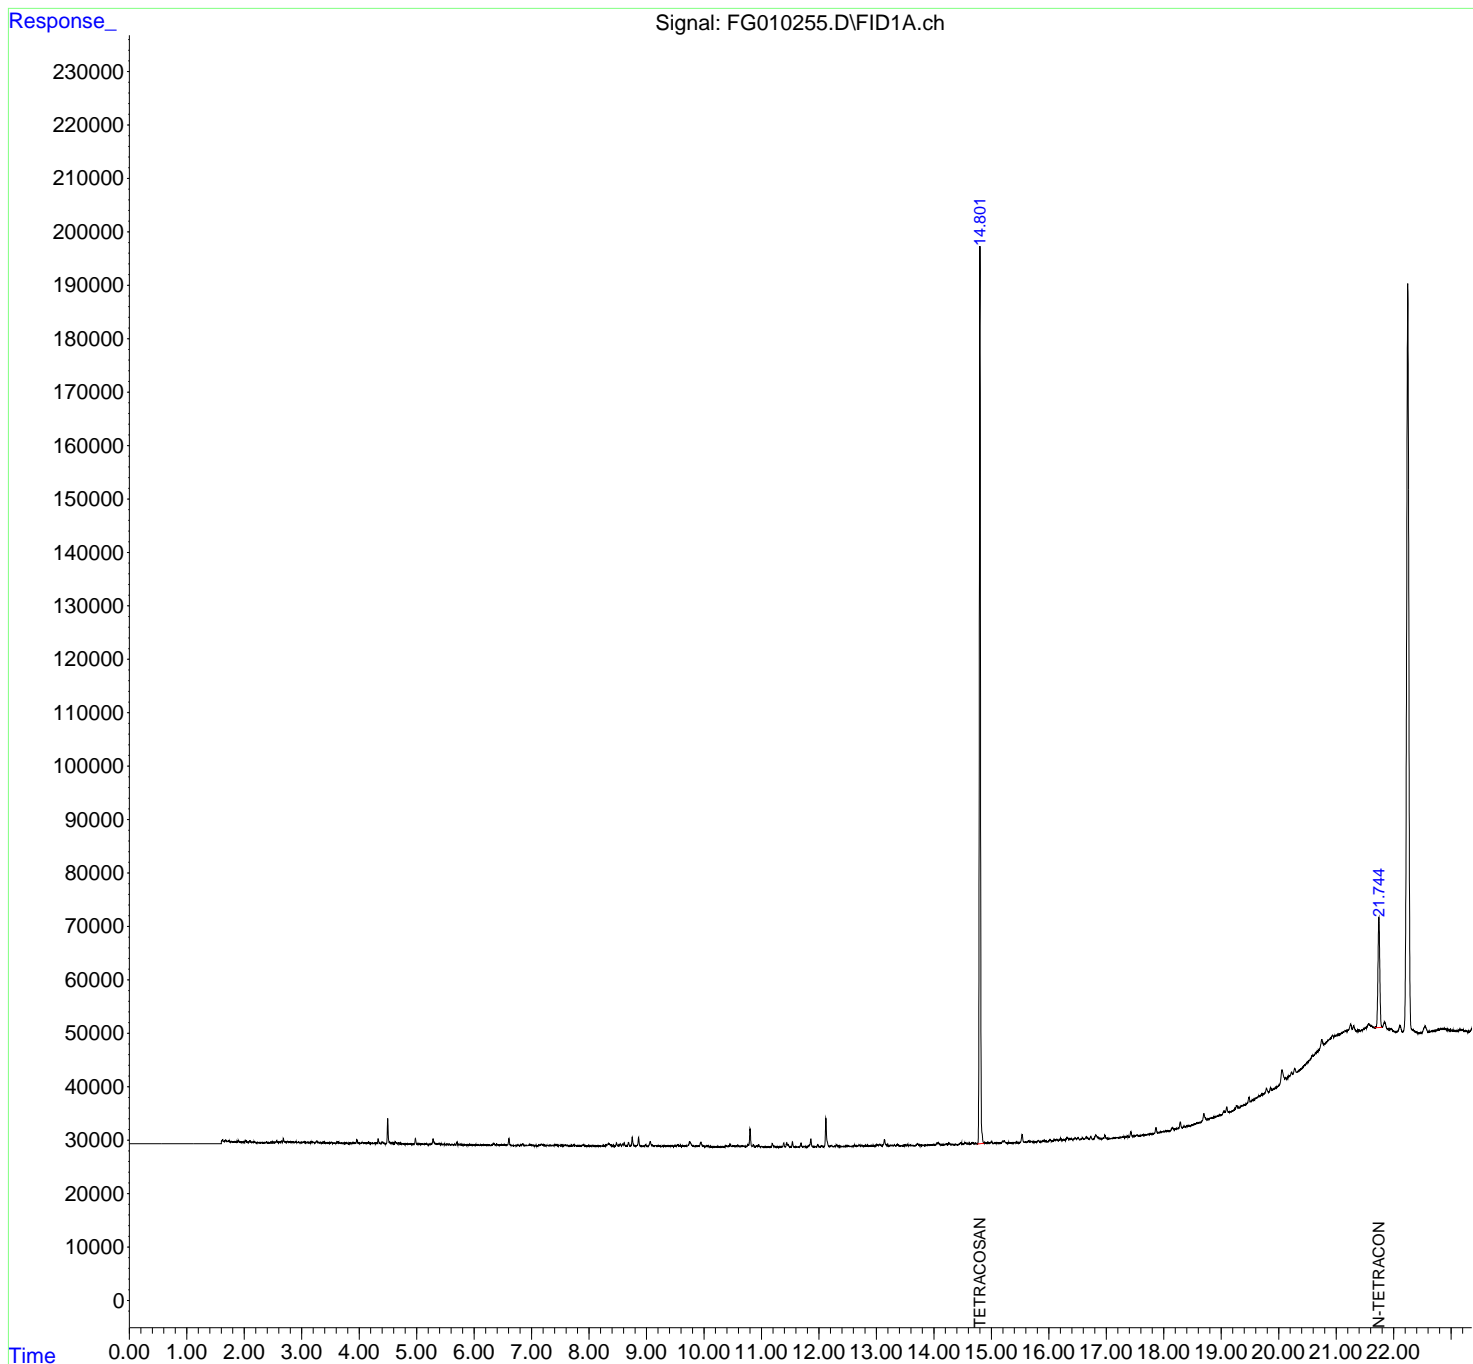


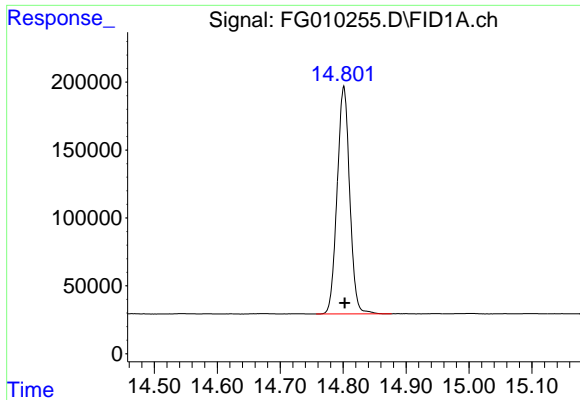

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.801 min
Delta R.T.: -0.001 min
Response: 2319982
Conc: 18.26 ug/ml

Instrument :
FID_G
ClientSampleId :

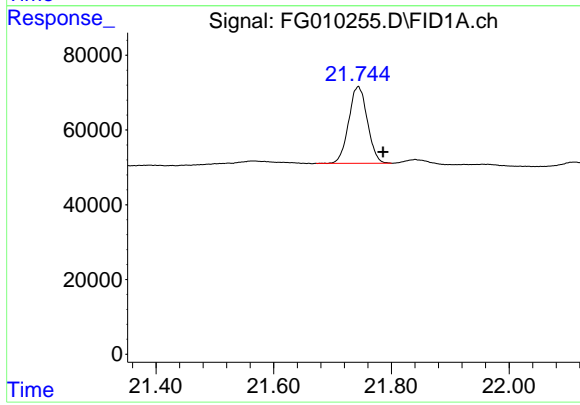

#18 N-TETRACONTANE

R.T.: 21.744 min
Delta R.T.: -0.042 min
Response: 452435
Conc: 3.86 ug/ml