

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG080124\
Data File : FG014019.D
Signal(s) : FID1A.ch
Acq On : 01 Aug 2024 16:48
Operator : YP\AJ
Sample : PB162386BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 02 05:35:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG072324.M
Quant Title :
QLast Update : Tue Jul 23 14:43:06 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.949	2069992	17.112 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.851	47866	0.392 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG080124\
Data File : FG014019.D
Signal(s) : FID1A.ch
Acq On : 01 Aug 2024 16:48
Operator : YP\AJ
Sample : PB162386BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 02 05:35:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG072324.M
Quant Title :
QLast Update : Tue Jul 23 14:43:06 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

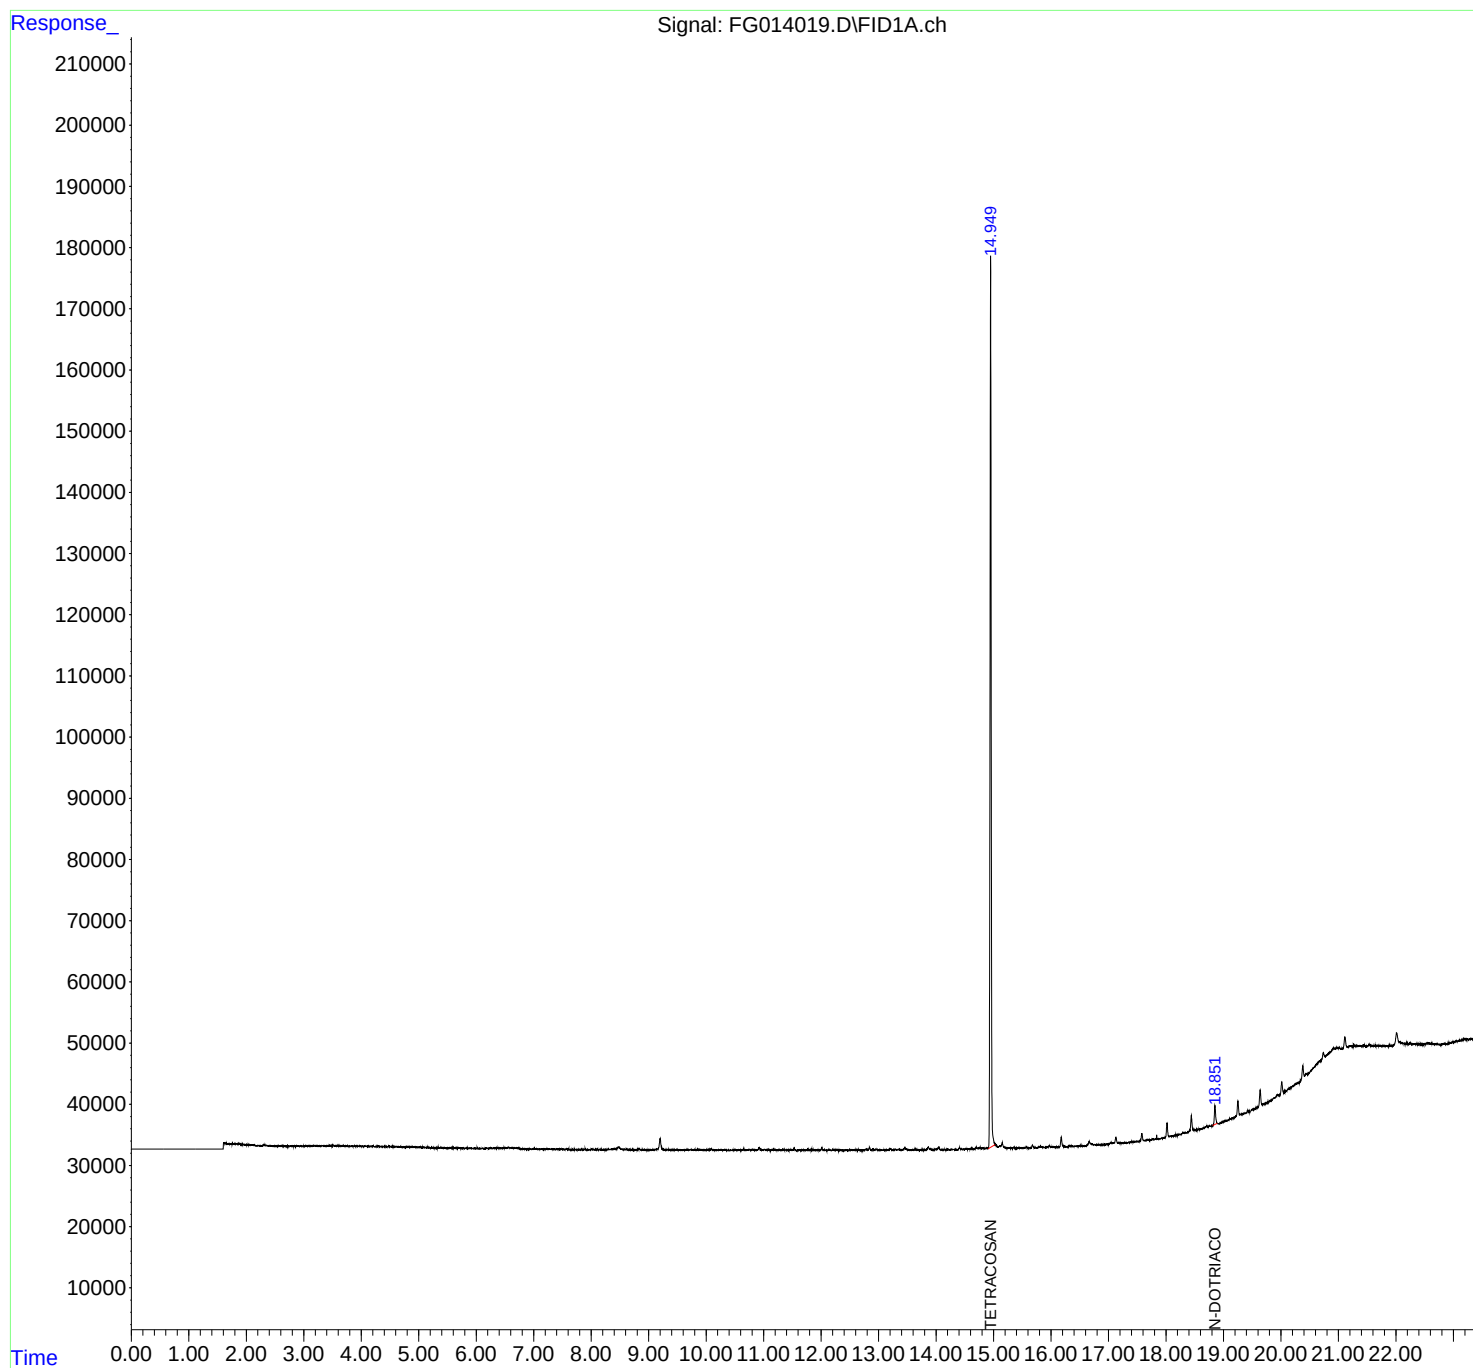

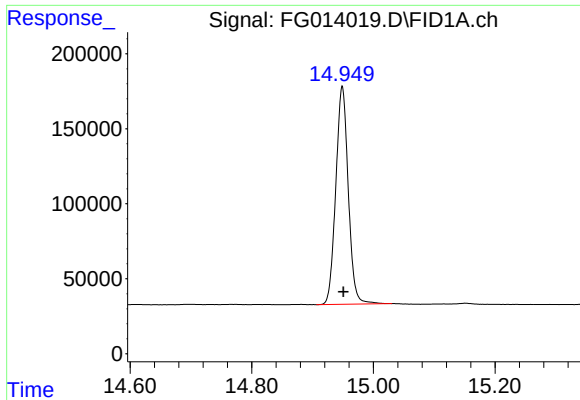

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.949 min
Delta R.T.: -0.002 min
Response: 2069992
Conc: 17.11 ug/ml

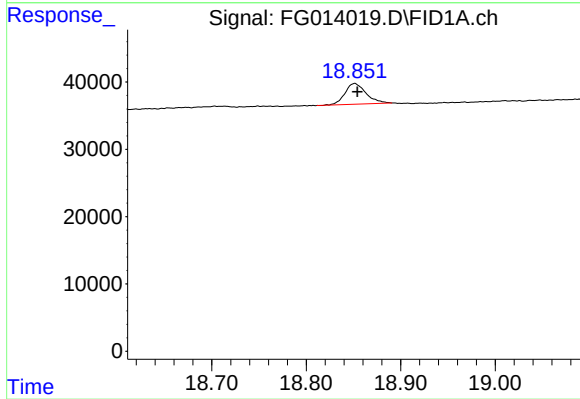

#14 N-DOTRIACONTANE

R.T.: 18.851 min
Delta R.T.: -0.003 min
Response: 47866
Conc: 0.39 ug/ml