

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG080224\
Data File : FG014047.D
Signal(s) : FID1A.ch
Acq On : 02 Aug 2024 18:30
Operator : YP\AJ
Sample : P3441-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
BU-02-08012024

Integration File: autoint1.e
Quant Time: Aug 03 01:43:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG072324.M
Quant Title :
QLast Update : Tue Jul 23 14:43:06 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.945	1728477	14.289 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG080224\
Data File : FG014047.D
Signal(s) : FID1A.ch
Acq On : 02 Aug 2024 18:30
Operator : YP\AJ
Sample : P3441-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
BU-02-08012024

Integration File: autoint1.e
Quant Time: Aug 03 01:43:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG072324.M
Quant Title :
QLast Update : Tue Jul 23 14:43:06 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

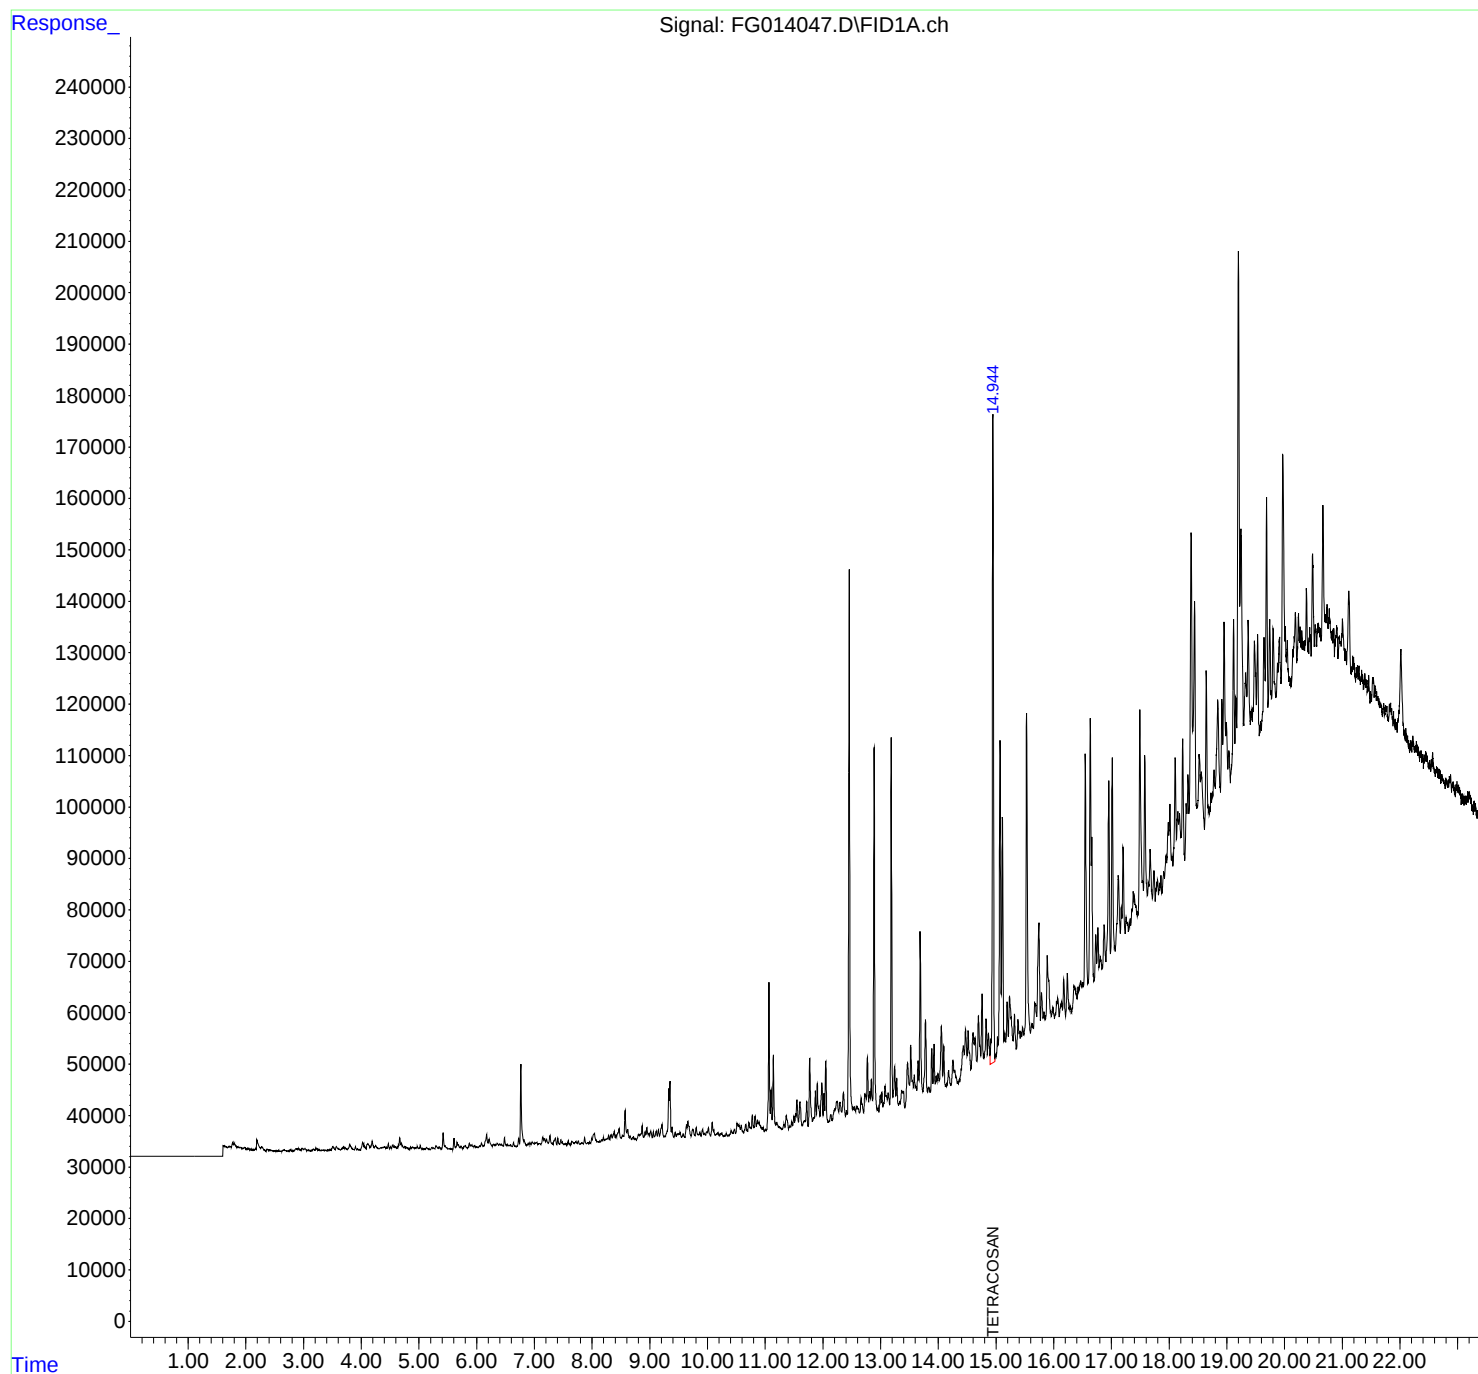

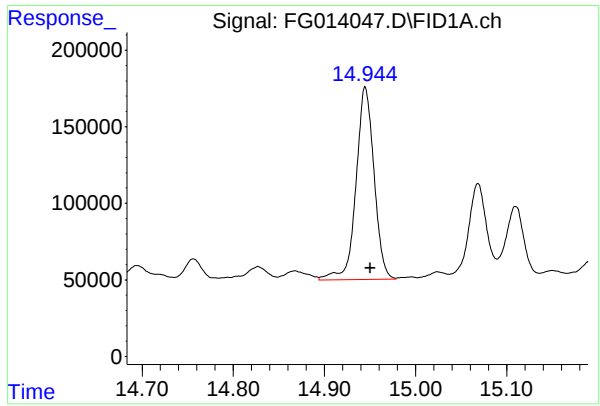

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.945 min
Delta R.T.: -0.006 min
Response: 1728477
Conc: 14.29 ug/ml

Instrument :
FID_G
ClientSampleId :
BU-02-08012024