

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG080618\
 Data File : FG001961.D
 Signal(s) : FID1A.ch
 Acq On : 06 Aug 2018 12:03
 Operator : AJ\SJ
 Sample : 4400 TRPH STD
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Aug 06 13:12:11 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\C44-FG080618.M
 Quant Title :
 QLast Update : Mon Aug 06 13:11:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.479	19665352	50.000 ug/ml
Target Compounds			
1) N-OCTANE	2.242	119649986	400.000 ug/ml
2) N-NONANE	3.224	121960249	400.000 ug/ml
3) N-DECANE	4.283	186926984	400.000 ug/ml
4) N-UNDECANE	5.311	188552451	600.000 ug/ml
5) N-DODECANE	6.289	188148478	600.000 ug/ml
6) N-TETRADECANE	8.083	190017343	600.000 ug/ml
7) N-HEXADECANE	9.678	158477498	500.000 ug/ml
8) N-OCTADECANE	11.098	78907794	250.000 ug/ml
9) N-EICOSANE	12.389	31348558	100.000 ug/ml
10) N-TETRACOSANE	14.689	30858856	100.000 ug/ml
11) N-OCTACOSANE	16.649	14890069	50.000 ug/ml
12) N-DOTRIACONTANE	18.369	13927407	50.000 ug/ml
14) N-HEXATRIACONTANE	19.894	12491899	50.000 ug/ml
15) N-TETRACONTANE	21.437	10266491	50.000 ug/ml
16) N-TETRTETRACOOCTANE	23.953	6599574	50.000 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG080618\
Data File : FG001961.D
Signal(s) : FID1A.ch
Acq On : 06 Aug 2018 12:03
Operator : AJ\SJ
Sample : 4400 TRPH STD
Misc :
ALS Vial : 4 Sample Multiplier: 1


Integration File: autoint1.e
Quant Time: Aug 06 13:12:11 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\C44-FG080618.M
Quant Title :
QLast Update : Mon Aug 06 13:11:38 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

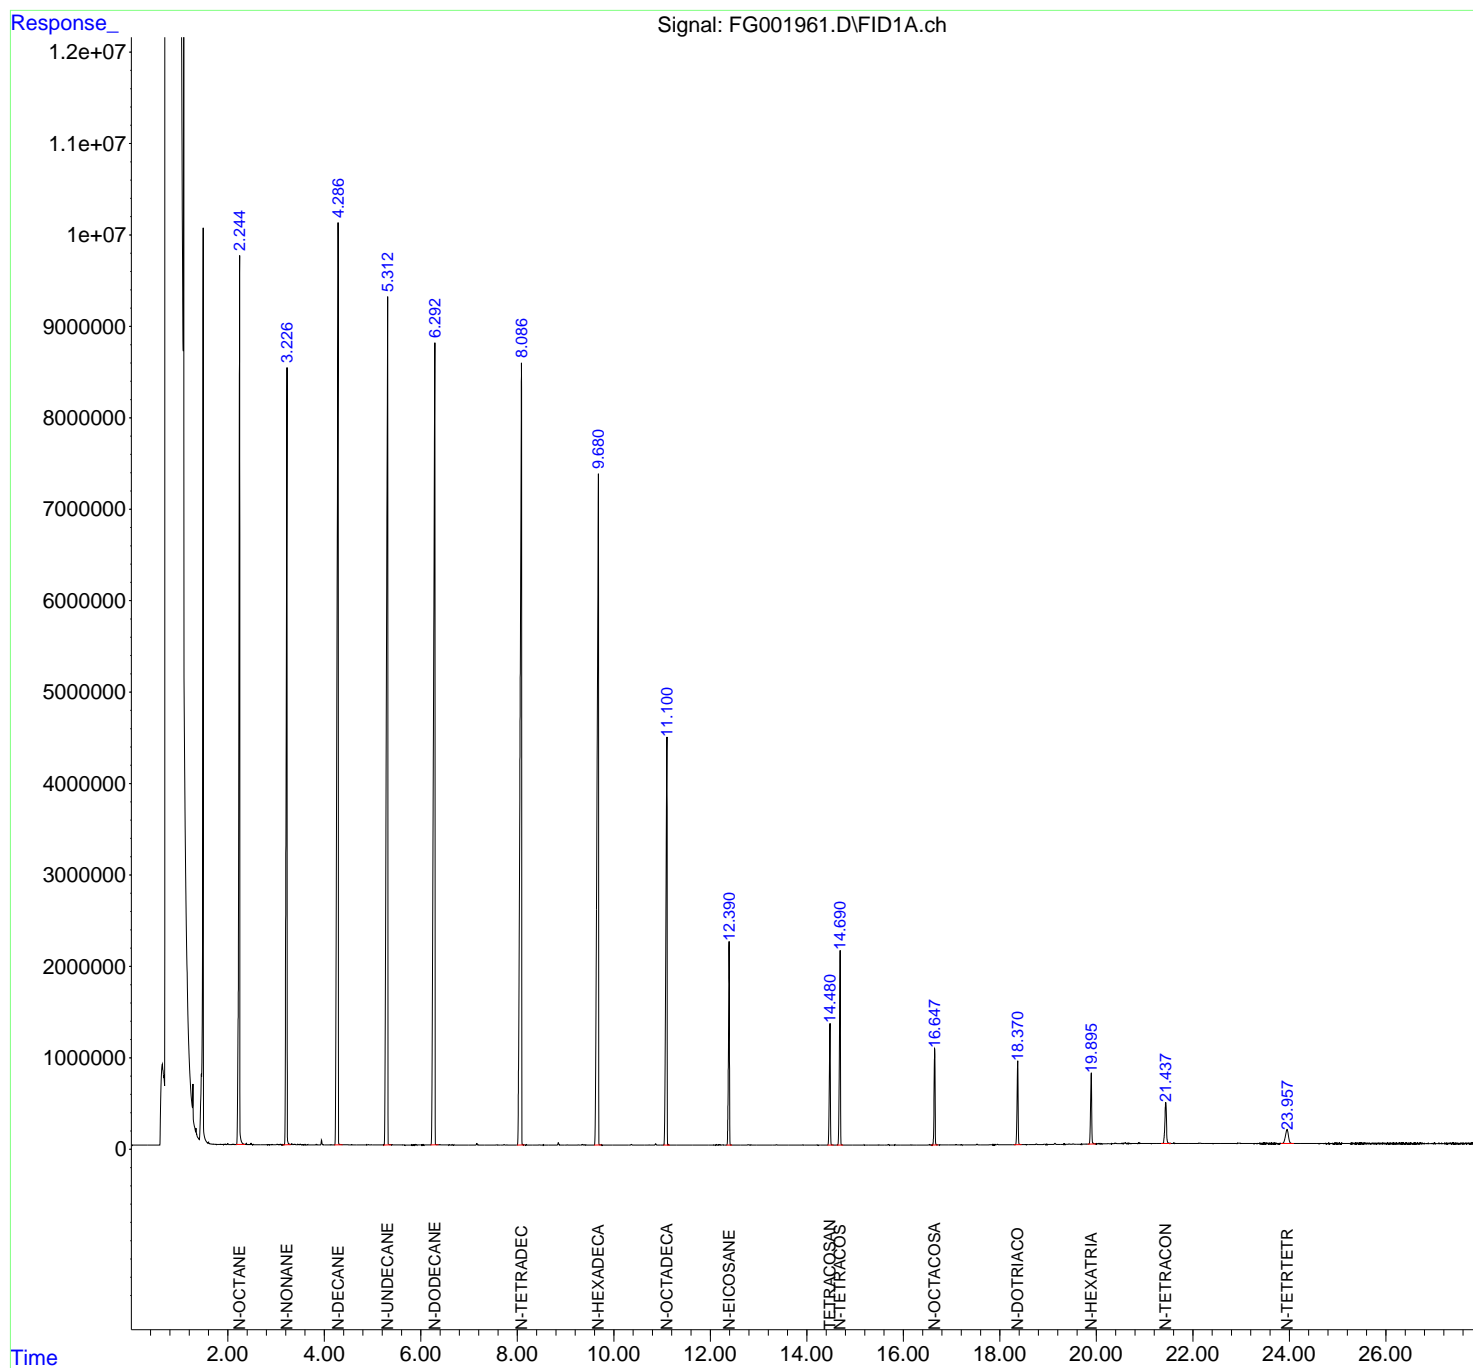


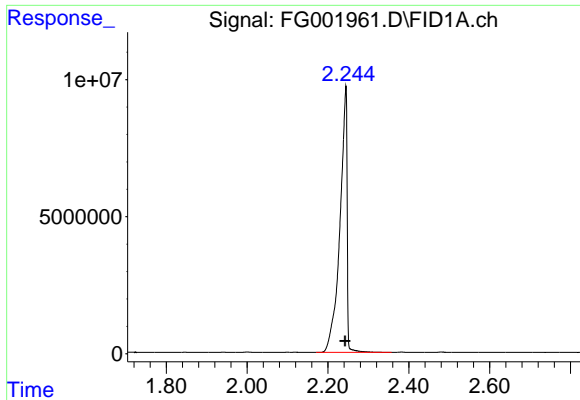


#1 N-OCTANE
R.T.: 2.242 min
Delta R.T.: 0.000 min
Response: 119649986
Conc: 400.00 ug/ml

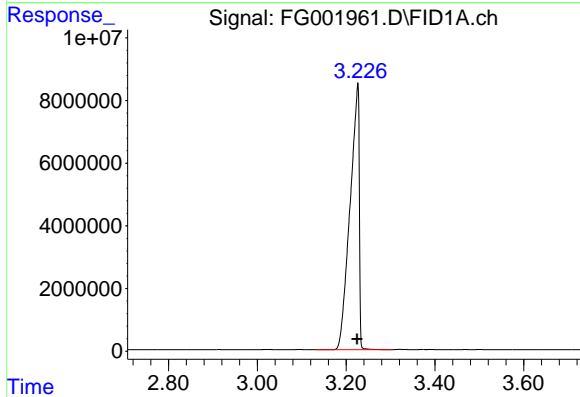


#2 N-NONANE
R.T.: 3.224 min
Delta R.T.: 0.000 min
Response: 121960249
Conc: 400.00 ug/ml

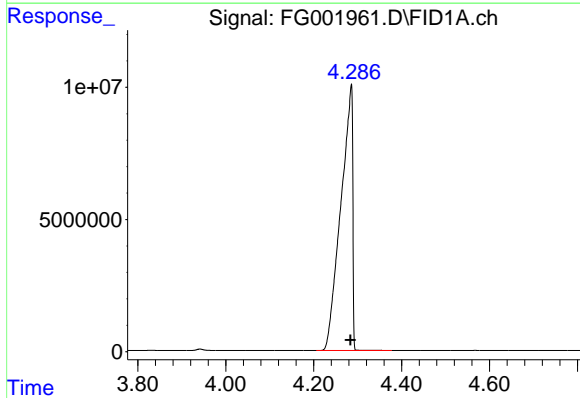

#3 N-DECANE
R.T.: 4.283 min
Delta R.T.: 0.000 min
Response: 186926984
Conc: 400.00 ug/ml

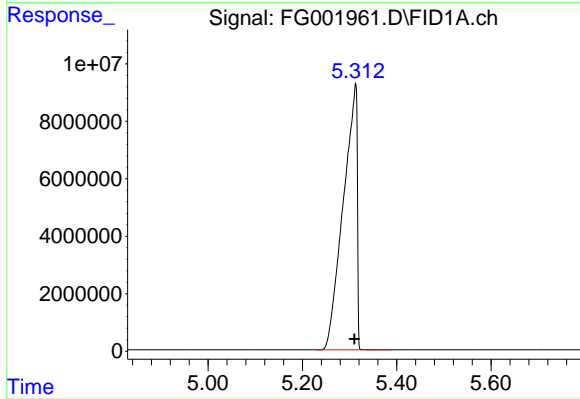


#4 N-UNDECANE
R.T.: 5.311 min
Delta R.T.: 0.000 min
Response: 188552451
Conc: 600.00 ug/ml

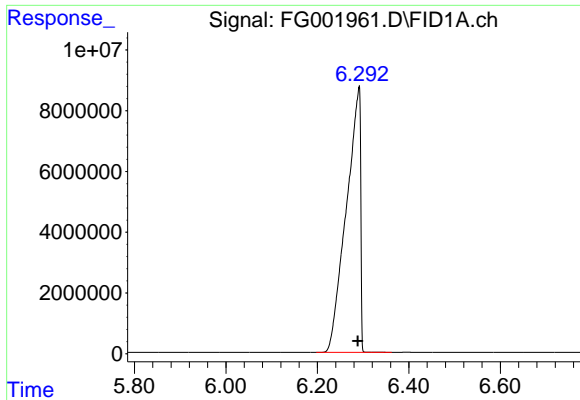


#5 N-DODECANE

R.T.: 6.289 min
Delta R.T.: 0.000 min
Response: 188148478
Conc: 600.00 ug/ml

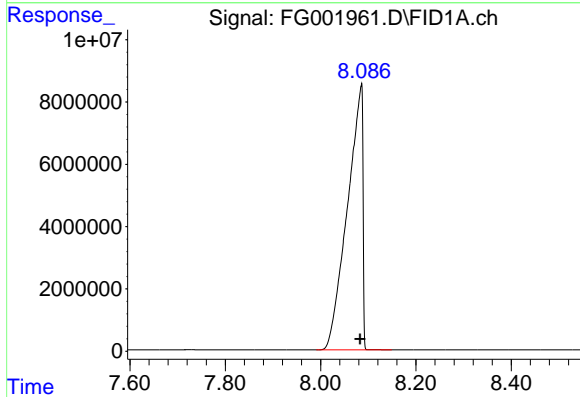


#6 N-TETRADECANE

R.T.: 8.083 min
Delta R.T.: 0.000 min
Response: 190017343
Conc: 600.00 ug/ml

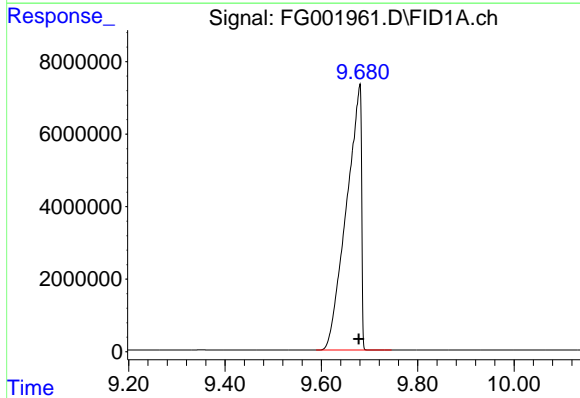


#7 N-HEXADECANE

R.T.: 9.678 min
Delta R.T.: 0.000 min
Response: 158477498
Conc: 500.00 ug/ml

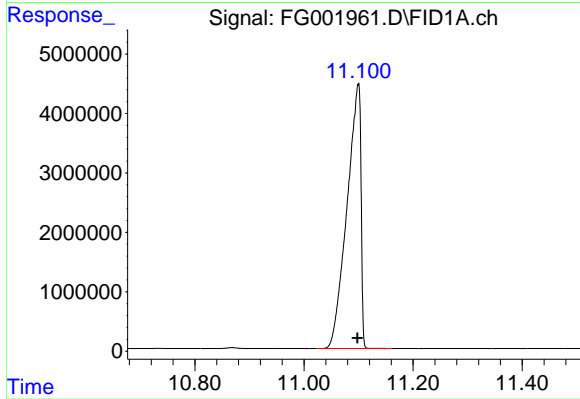


#8 N-OCTADECANE

R.T.: 11.098 min
Delta R.T.: 0.000 min
Response: 78907794
Conc: 250.00 ug/ml

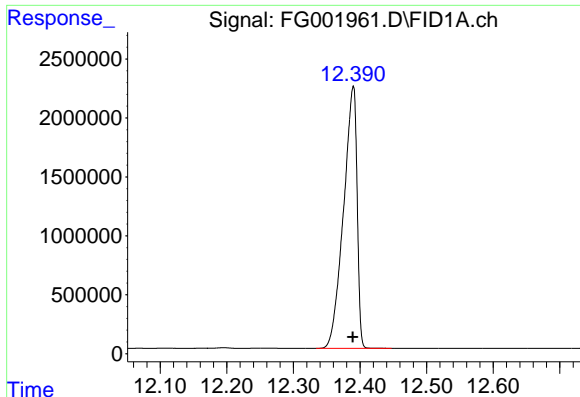


#9 N-EICOSANE

R.T.: 12.389 min
Delta R.T.: 0.000 min
Response: 31348558
Conc: 100.00 ug/ml

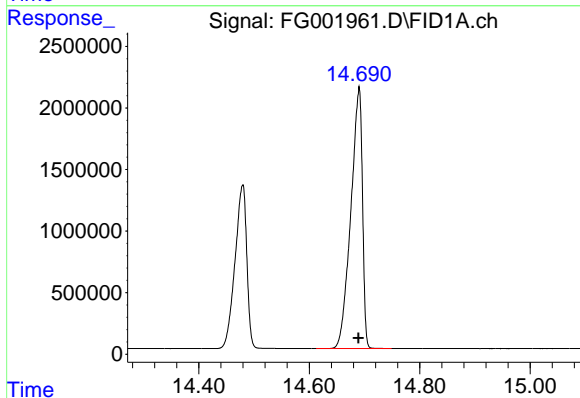


#10 N-TETRACOSANE

R.T.: 14.689 min
Delta R.T.: 0.000 min
Response: 30858856
Conc: 100.00 ug/ml

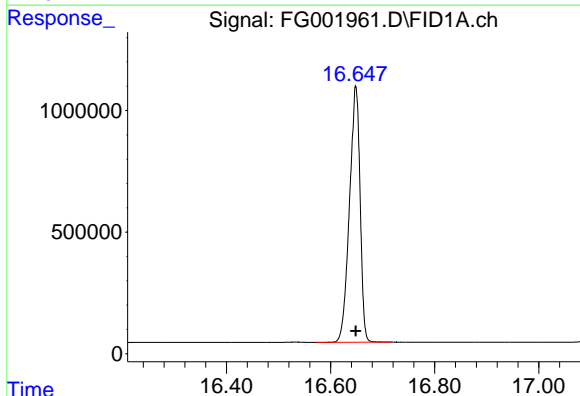


#11 N-OCTACOSANE

R.T.: 16.649 min
Delta R.T.: 0.000 min
Response: 14890069
Conc: 50.00 ug/ml

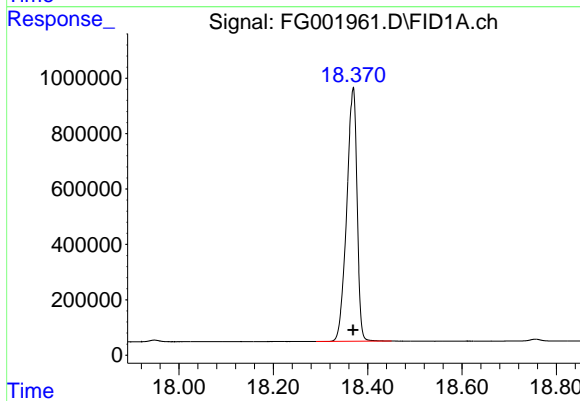


#12 N-DOTRIACONTANE

R.T.: 18.369 min
Delta R.T.: 0.000 min
Response: 13927407
Conc: 50.00 ug/ml

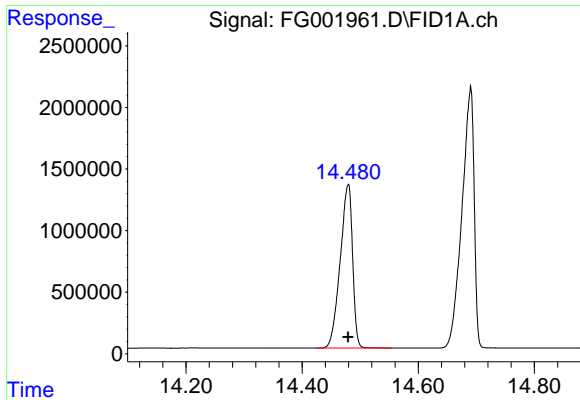


#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.479 min
Delta R.T.: 0.000 min
Response: 19665352
Conc: 50.00 ug/ml

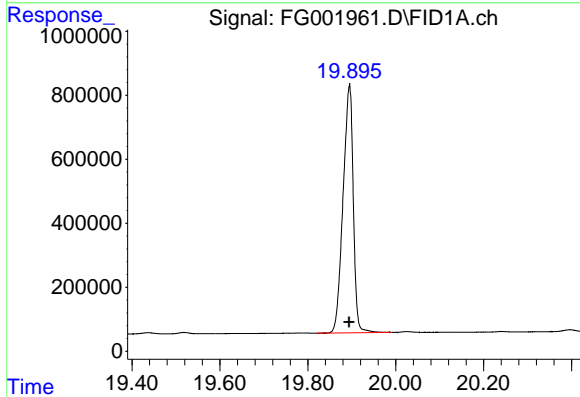


#14 N-HEXATRIACONTANE

R.T.: 19.894 min
Delta R.T.: 0.000 min
Response: 12491899
Conc: 50.00 ug/ml

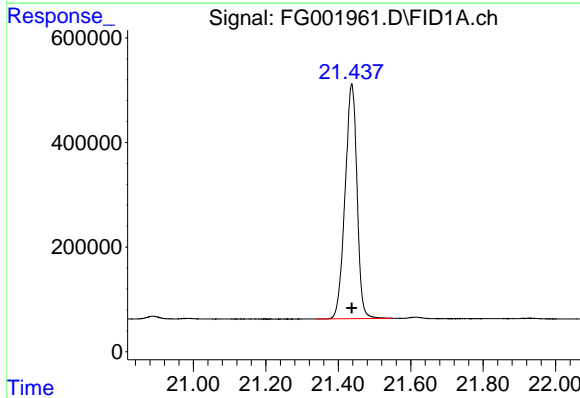

#15 N-TETRACONTANE

R.T.: 21.437 min
Delta R.T.: 0.000 min
Response: 10266491
Conc: 50.00 ug/ml

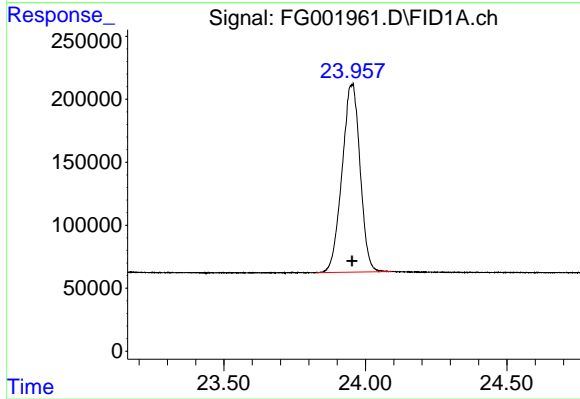

#16 N-TETRTETRAOCTANE

R.T.: 23.953 min
Delta R.T.: 0.000 min
Response: 6599574
Conc: 50.00 ug/ml