

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG080621\
 Data File : FG080576.D
 Signal(s) : FID1A.ch
 Acq On : 06 Aug 2021 20:16
 Operator : DD\AJ
 Sample : M3281-01 400X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 09 02:01:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG071521.M
 Quant Title :
 QLast Update : Thu Jul 15 13:17:03 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.510	279378	1.815 ug/ml
4) N-TETRADECANE	8.279	342193	2.196 ug/ml
5) N-HEXADECANE	9.901	158287	1.020 ug/ml
13) N-TRIACONTANE	17.832	26266	0.166 ug/ml
14) N-DOTRIACONTANE	18.664	481670	3.206 ug/ml
16) N-HEXATRIACONTANE	20.188	77991	0.662 ug/ml
17) N-OCTATRIACONTANE	20.967	119990	1.203 ug/ml
18) N-TETRACONTANE	21.897	4904	0.054 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG080621\
Data File : FG008576.D
Signal(s) : FID1A.ch
Acq On : 06 Aug 2021 20:16
Operator : DD\AJ
Sample : M3281-01 400X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampled :

Integration File: autoint1.e
Quant Time: Aug 09 02:01:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG071521.M
Quant Title :
QLast Update : Thu Jul 15 13:17:03 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

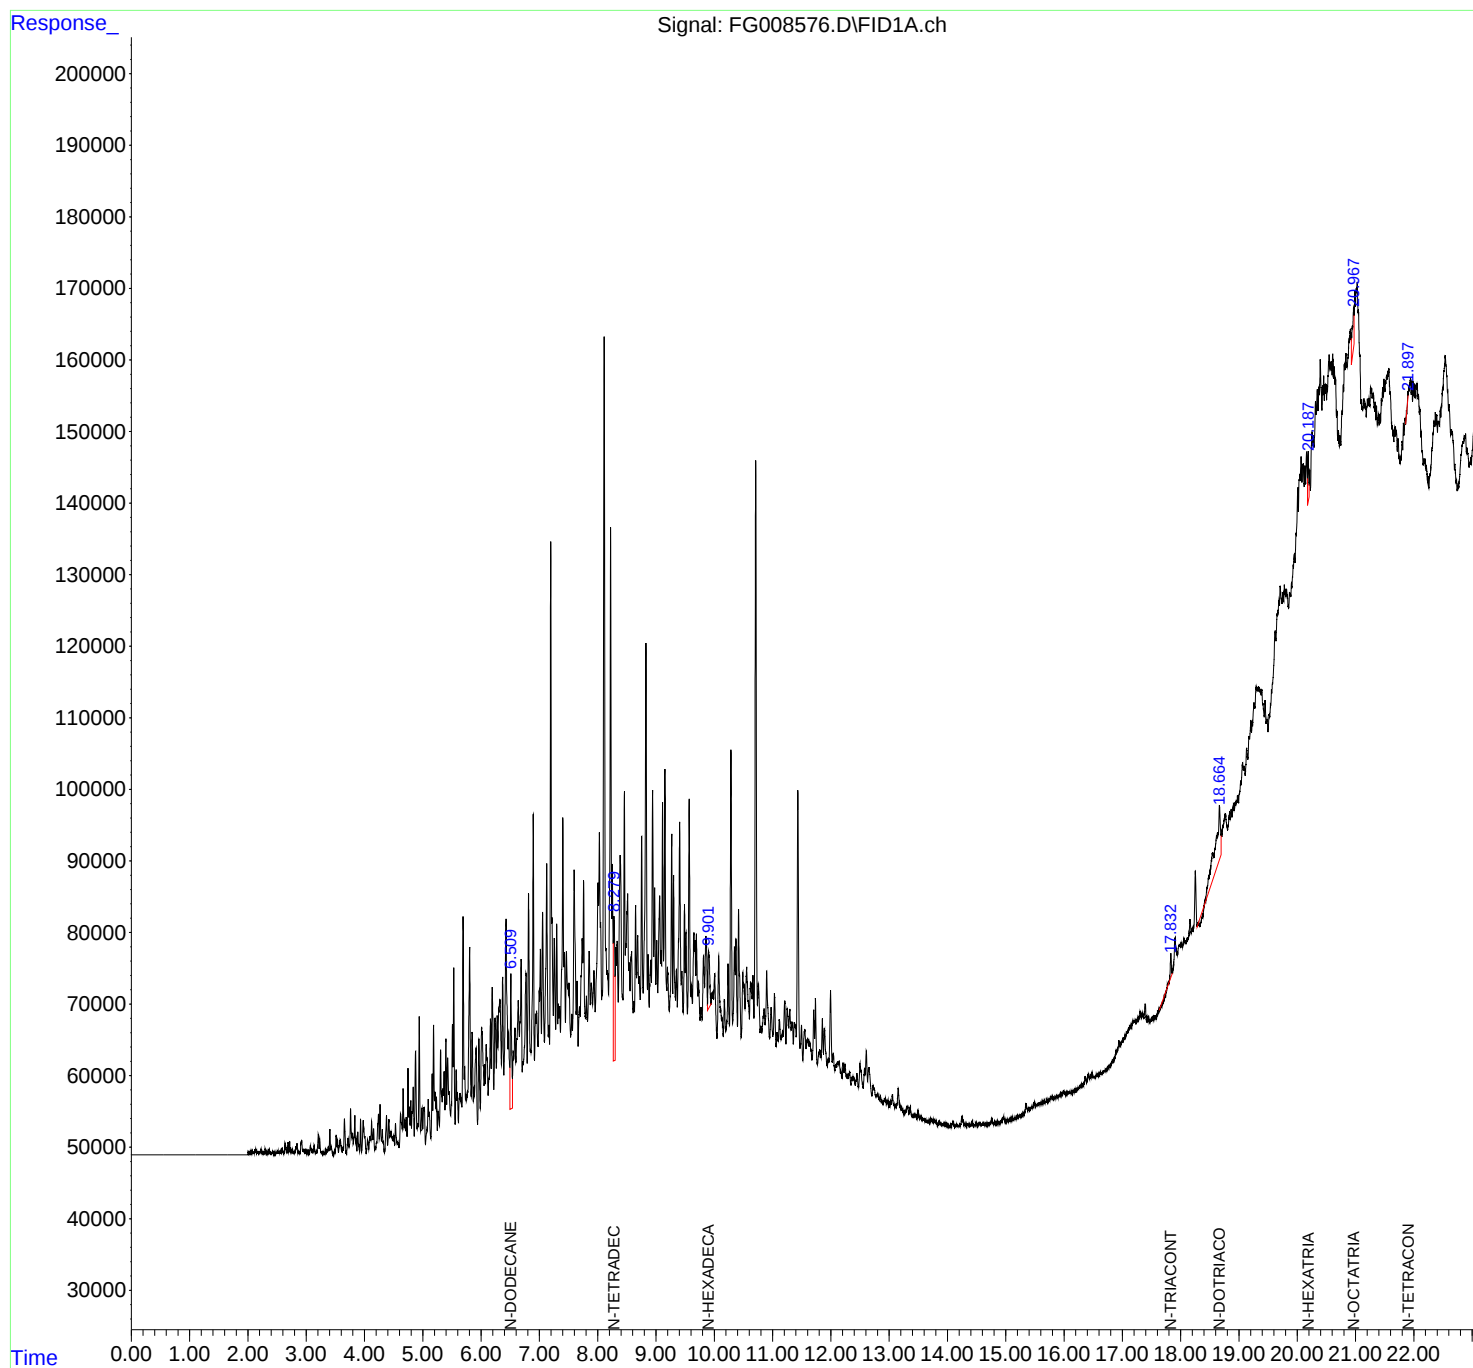


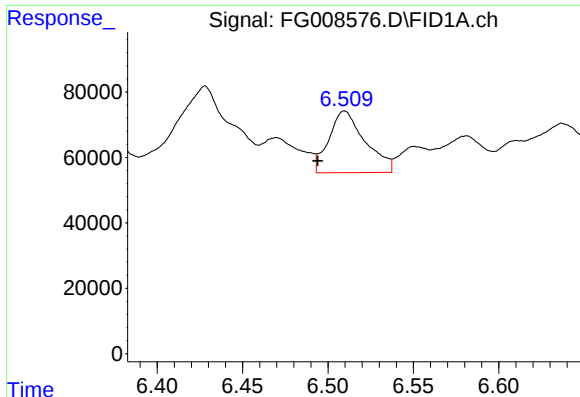

#3 N-DODECANE


R.T.: 6.510 min
Delta R.T.: 0.016 min
Response: 279378
Conc: 1.82 ug/ml

Instrument :
FID_G
ClientSampleId :

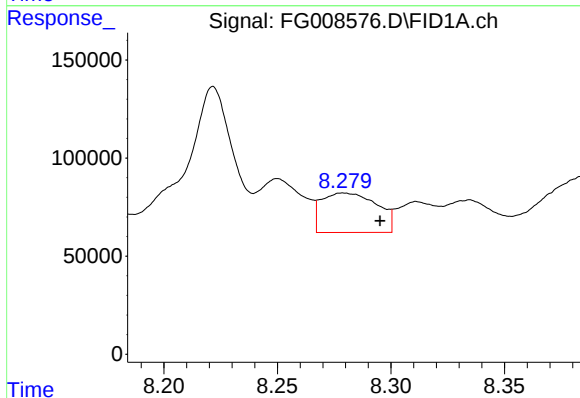


#4 N-TETRADECANE

R.T.: 8.279 min
Delta R.T.: -0.016 min
Response: 342193
Conc: 2.20 ug/ml

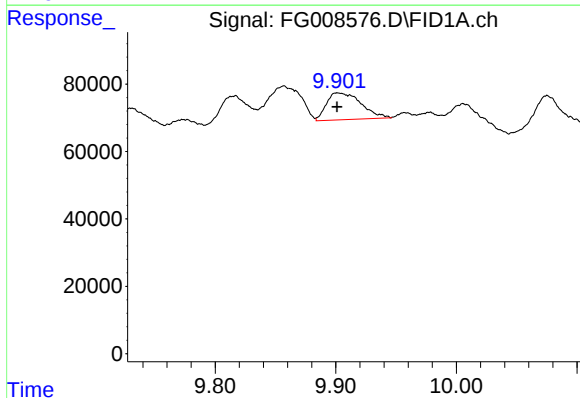


#5 N-HEXADECANE

R.T.: 9.901 min
Delta R.T.: 0.000 min
Response: 158287
Conc: 1.02 ug/ml

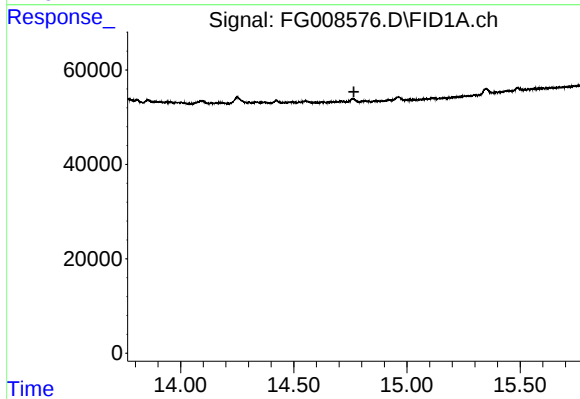

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.765 min
Response: 0
Conc: N.D.

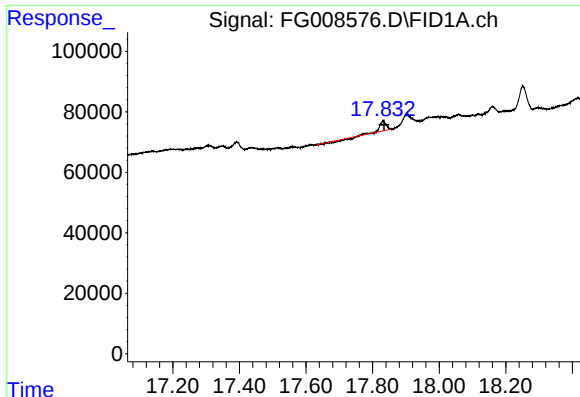

#13 N-TRIACONTANE


R.T.: 17.832 min
Delta R.T.: -0.003 min
Response: 26266
Conc: 0.17 ug/ml

Instrument :
FID_G
ClientSampleId :

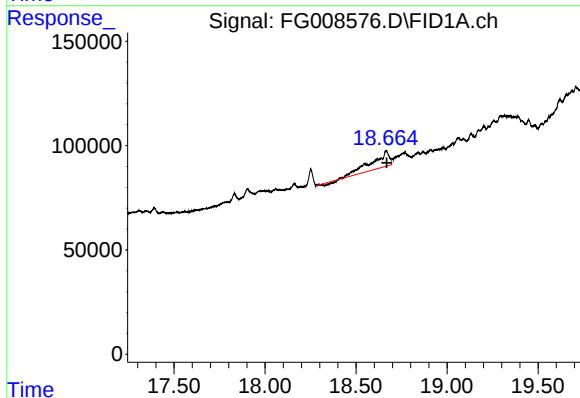


#14 N-DOTRIACONTANE

R.T.: 18.664 min
Delta R.T.: -0.005 min
Response: 481670
Conc: 3.21 ug/ml

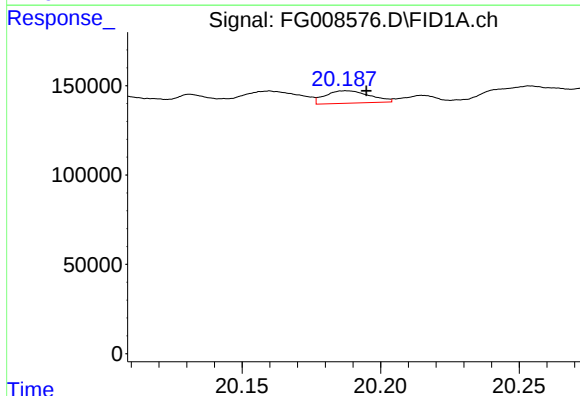


#16 N-HEXATRIACONTANE

R.T.: 20.188 min
Delta R.T.: -0.007 min
Response: 77991
Conc: 0.66 ug/ml

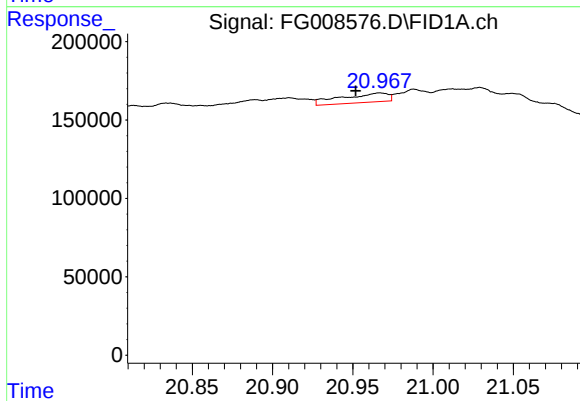

#17 N-OCTATRIACONTANE

R.T.: 20.967 min
Delta R.T.: 0.015 min
Response: 119990
Conc: 1.20 ug/ml

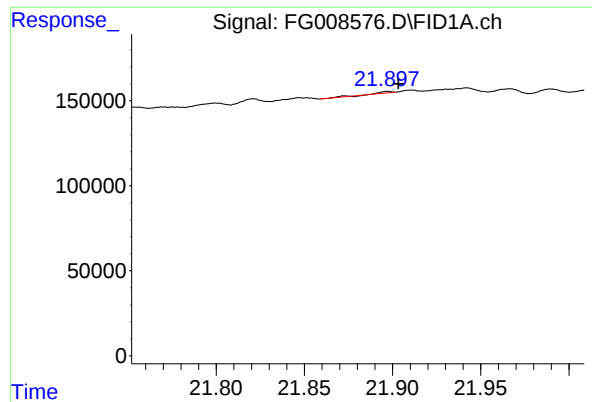

#18 N-TETRACONTANE

R.T.: 21.897 min
Delta R.T.: -0.006 min
Response: 4904
Conc: 0.05 ug/ml

Instrument :
FID_G
ClientSampleId :