

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG080621\  
Data File : FG080577.D  
Signal(s) : FID1A.ch  
Acq On : 06 Aug 2021 21:51  
Operator : DD\AJ  
Sample : MECL2  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Aug 09 02:01:54 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG071521.M  
Quant Title :  
QLast Update : Thu Jul 15 13:17:03 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    |                    | R.T.   | Response | Conc Units  |
|-----------------------------|--------------------|--------|----------|-------------|
| -----                       |                    |        |          |             |
| System Monitoring Compounds |                    |        |          |             |
| Target Compounds            |                    |        |          |             |
| 13)                         | N-TRIACONTANE      | 17.829 | 93263    | 0.590 ug/ml |
| 14)                         | N-DOTRIACONTANE    | 18.664 | 125341   | 0.834 ug/ml |
| 15)                         | N-TETRATRIACONTANE | 19.450 | 104072   | 0.755 ug/ml |
| 16)                         | N-HEXATRIACONTANE  | 20.191 | 418149   | 3.549 ug/ml |
| -----                       |                    |        |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG080621\  
Data File : FG008577.D  
Signal(s) : FID1A.ch  
Acq On : 06 Aug 2021 21:51  
Operator : DD\AJ  
Sample : MECL2  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampled :

Integration File: autoint1.e  
Quant Time: Aug 09 02:01:54 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG071521.M  
Quant Title :  
QLast Update : Thu Jul 15 13:17:03 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

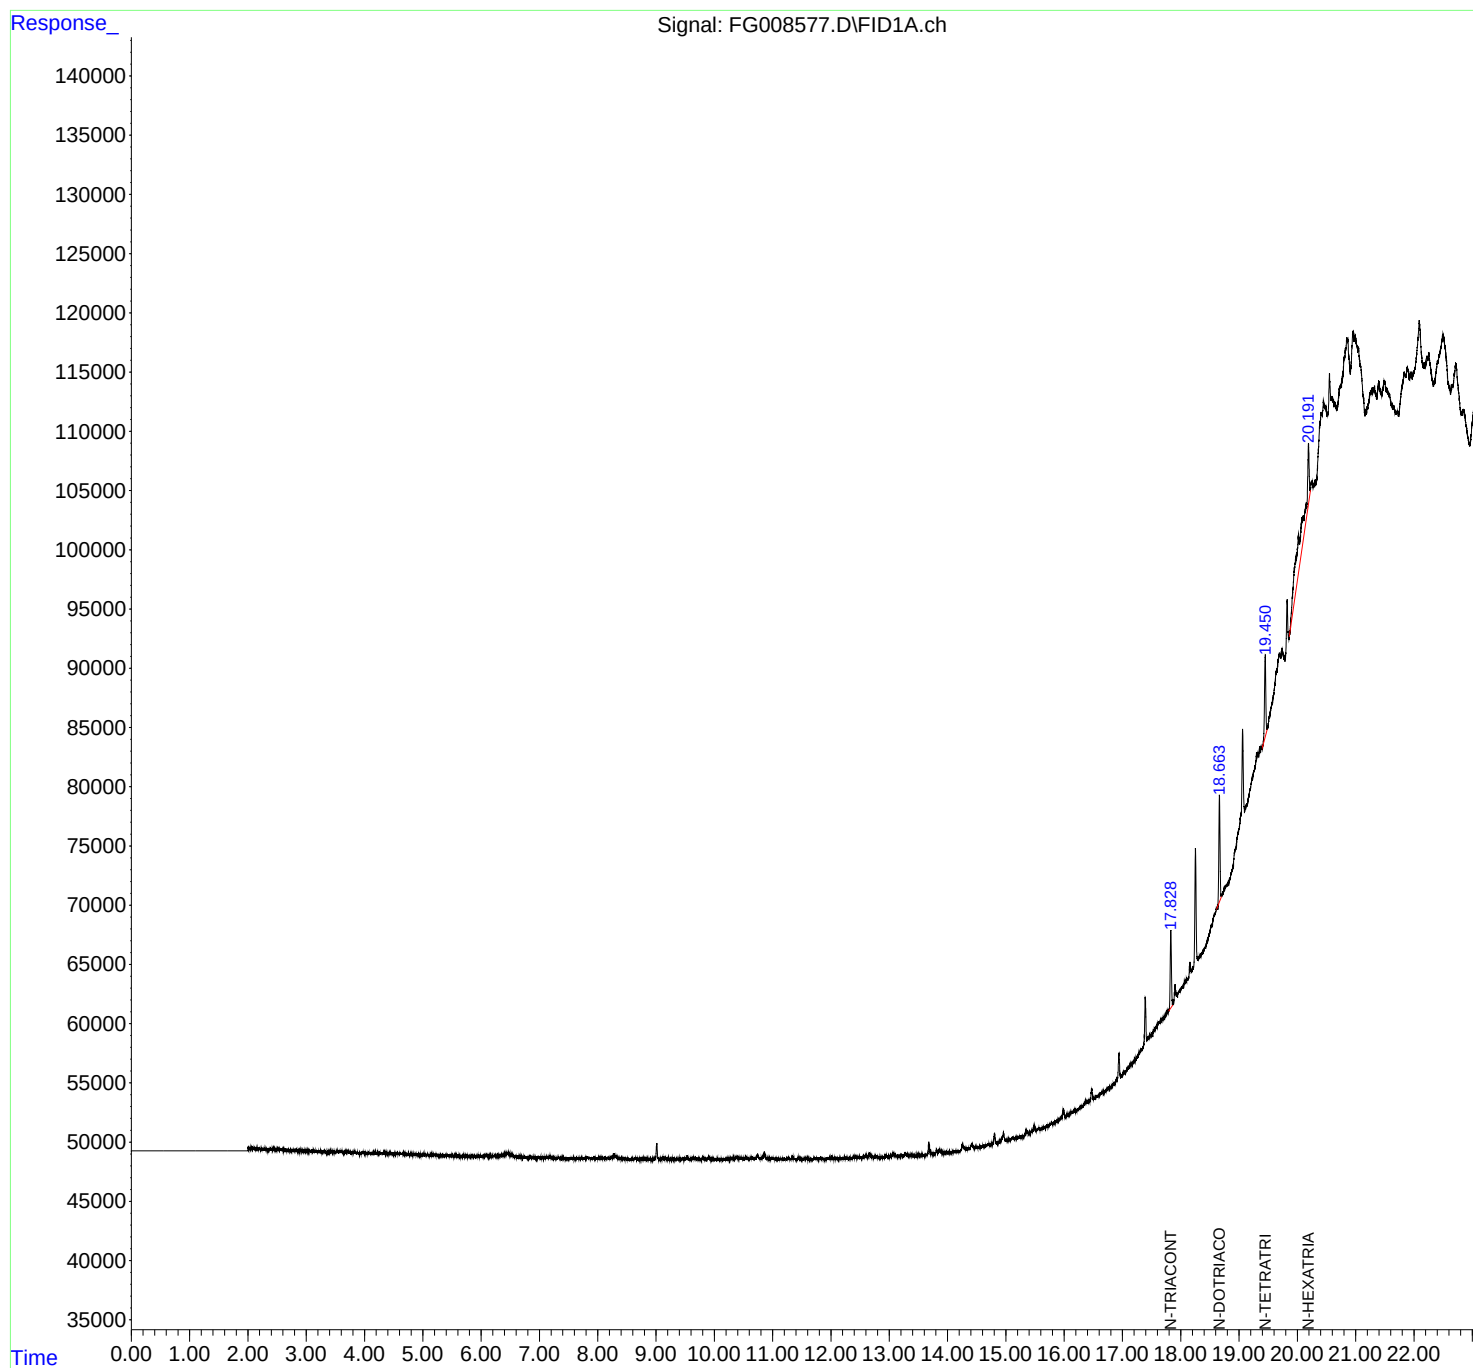


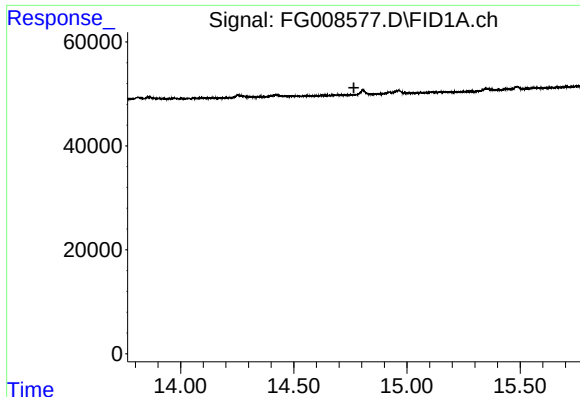

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min  
Exp R.T.: 14.765 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_G  
ClientSampleId :

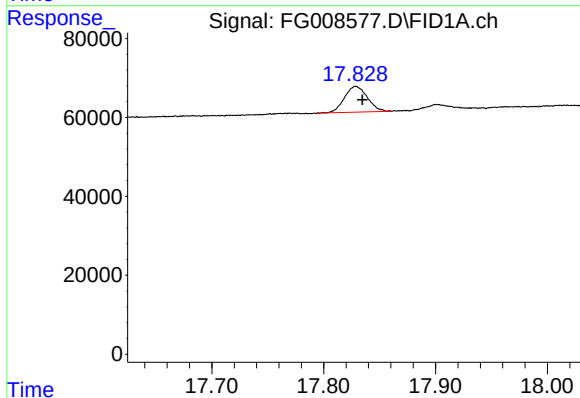


#13 N-TRIACONTANE

R.T.: 17.829 min  
Delta R.T.: -0.006 min  
Response: 93263  
Conc: 0.59 ug/ml

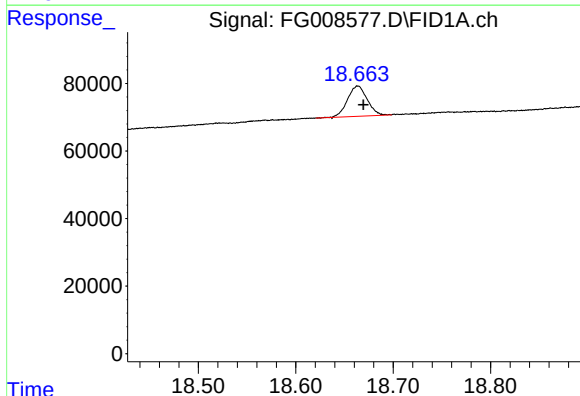


#14 N-DOTRIACONTANE

R.T.: 18.664 min  
Delta R.T.: -0.006 min  
Response: 125341  
Conc: 0.83 ug/ml

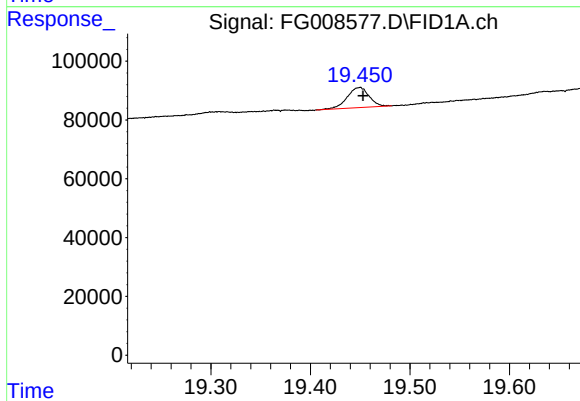

#15 N-TETRATRIACONTANE

R.T.: 19.450 min  
Delta R.T.: -0.003 min  
Response: 104072  
Conc: 0.76 ug/ml

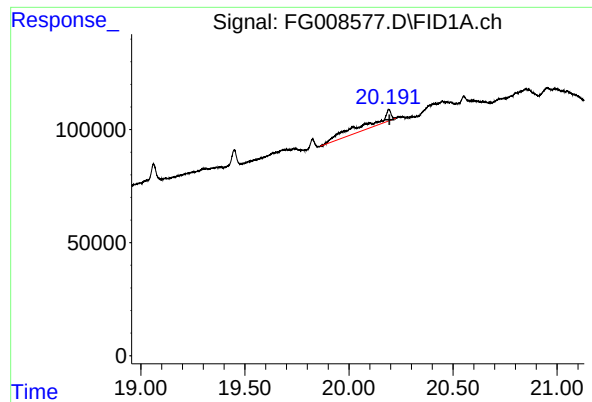

#16 N-HEXATRIACONTANE

R.T.: 20.191 min  
Delta R.T.: -0.003 min  
Response: 418149  
Conc: 3.55 ug/ml

Instrument :  
FID\_G  
ClientSampleId :