

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080718\
 Data File : FF001722.D
 Signal(s) : FID2B.ch
 Acq On : 07 Aug 2018 16:23
 Operator : AJ\SJ
 Sample : J4309-09
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Aug 08 00:57:43 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF080418.M
 Quant Title :
 QLast Update : Mon Aug 06 12:04:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.335	6731000	16.698 ug/ml
Target Compounds			
6) N-TETRADECANE	7.967	1903031	6.098 ug/ml
7) N-HEXADECANE	9.500	399265	1.268 ug/ml
8) N-OCTADECANE	10.982	1531622	4.856 ug/ml
9) N-EICOSANE	12.238	748012	2.371 ug/ml
10) N-TETRACOSANE	14.579	551190	1.735 ug/ml
11) N-OCTACOSANE	16.513	2612956	8.120 ug/ml
12) N-DOTRIACONTANE	18.185	6130946	18.791 ug/ml
14) N-HEXATRIACONTANE	19.739	1037594	3.517 ug/ml
15) N-TETRACONTANE	21.233	835734	3.471 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080718\
Data File : FF001722.D
Signal(s) : FID2B.ch
Acq On : 07 Aug 2018 16:23
Operator : AJ\SJ
Sample : J4309-09
Misc :
ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 08 00:57:43 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF080418.M
Quant Title :
QLast Update : Mon Aug 06 12:04:39 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

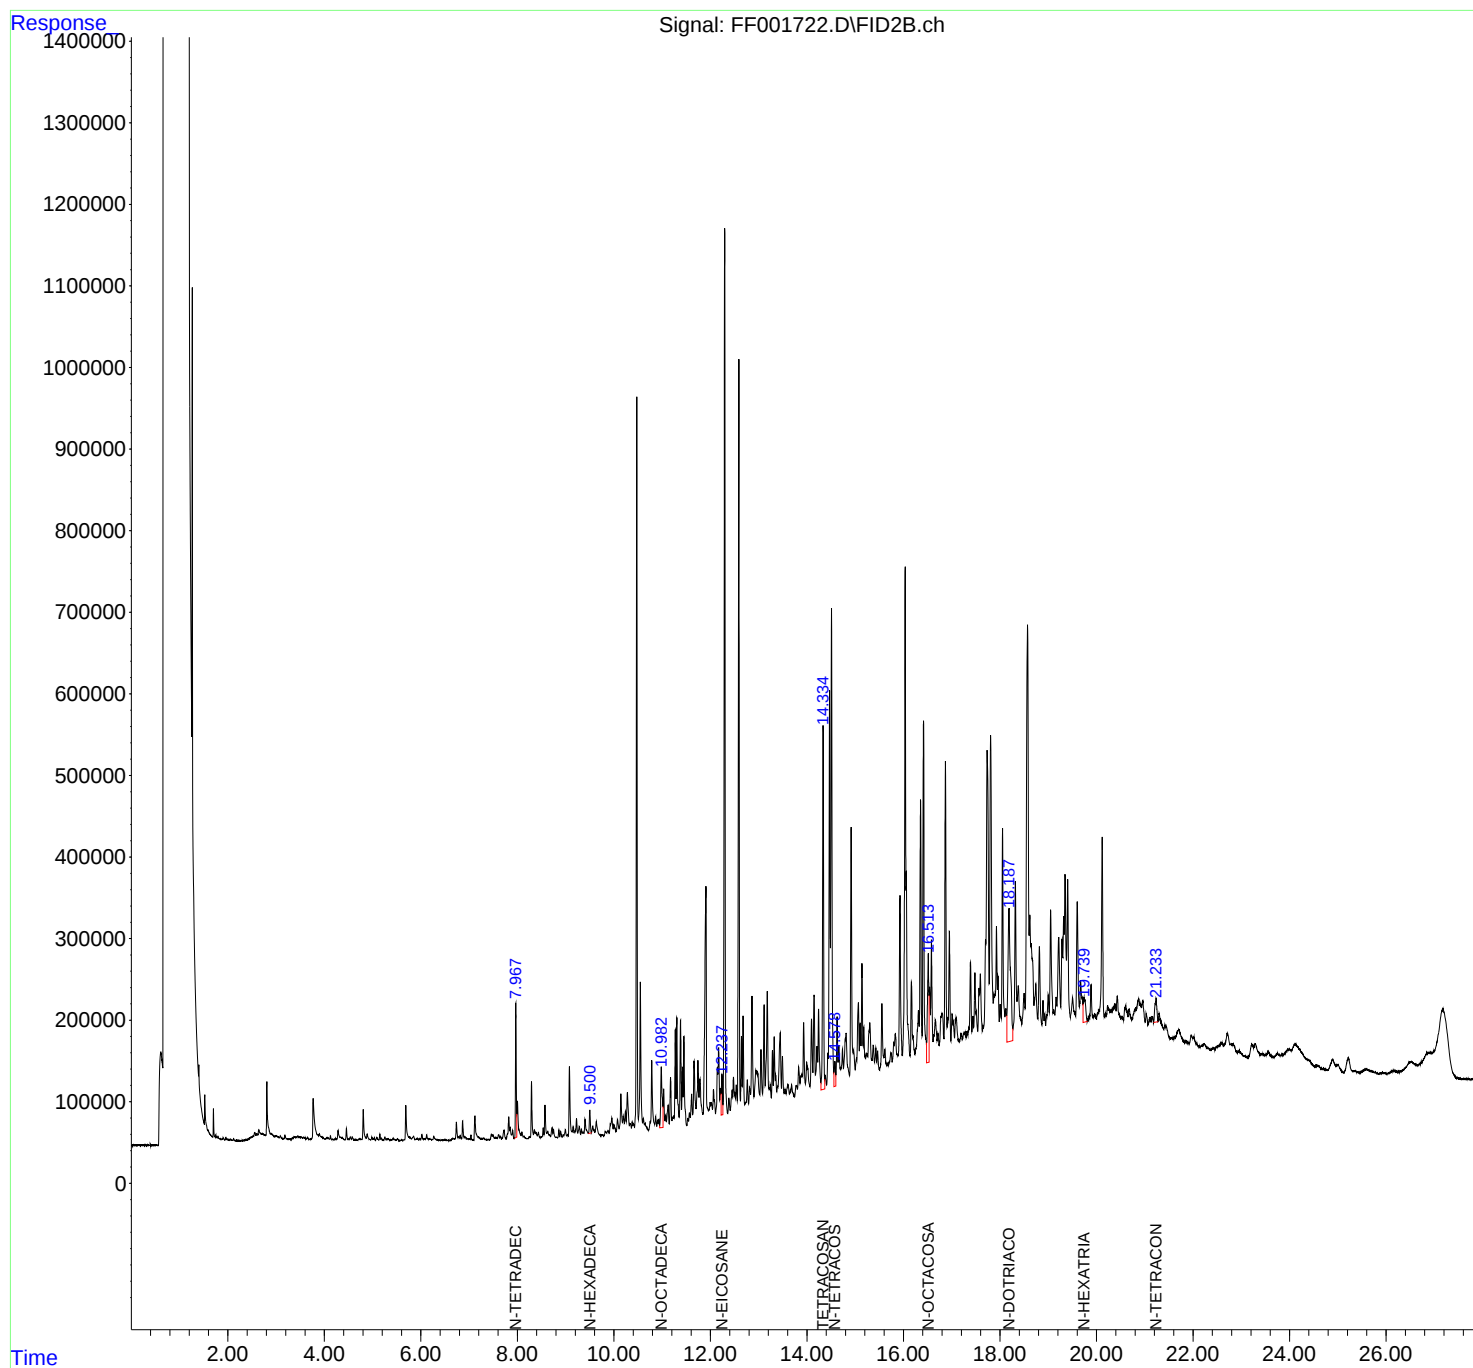

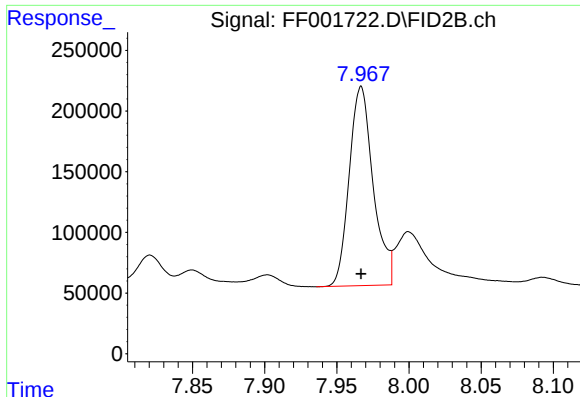


#6 N-TETRADECANE

R.T.: 7.967 min
Delta R.T.: 0.000 min
Response: 1903031
Conc: 6.10 ug/ml

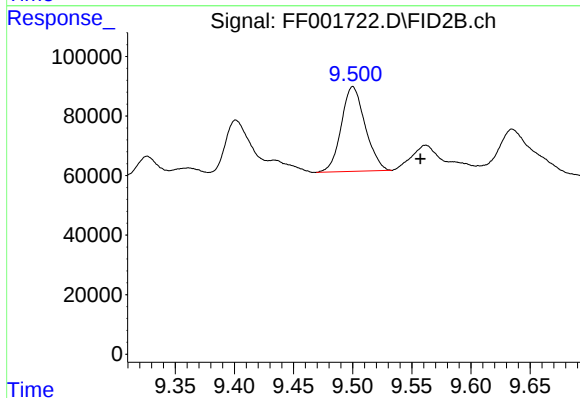


#7 N-HEXADECANE

R.T.: 9.500 min
Delta R.T.: -0.057 min
Response: 399265
Conc: 1.27 ug/ml

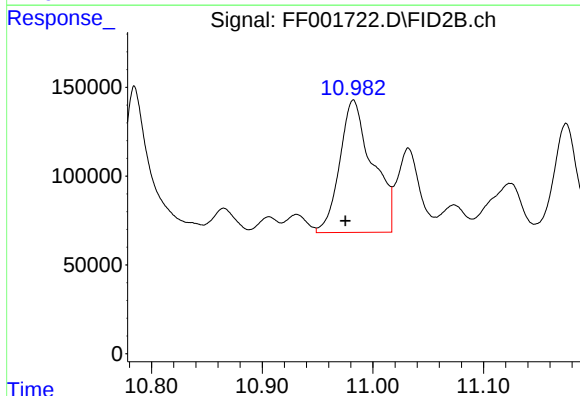


#8 N-OCTADECANE

R.T.: 10.982 min
Delta R.T.: 0.007 min
Response: 1531622
Conc: 4.86 ug/ml

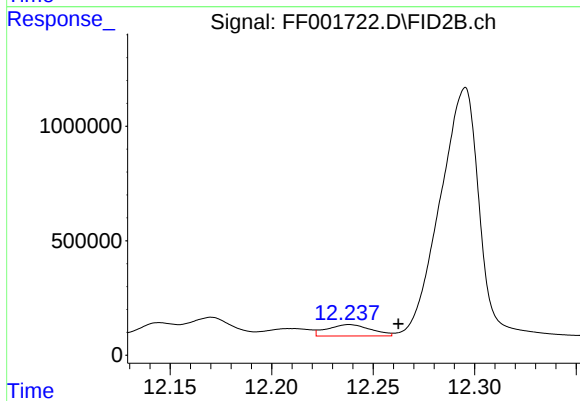


#9 N-EICOSANE

R.T.: 12.238 min
Delta R.T.: -0.024 min
Response: 748012
Conc: 2.37 ug/ml

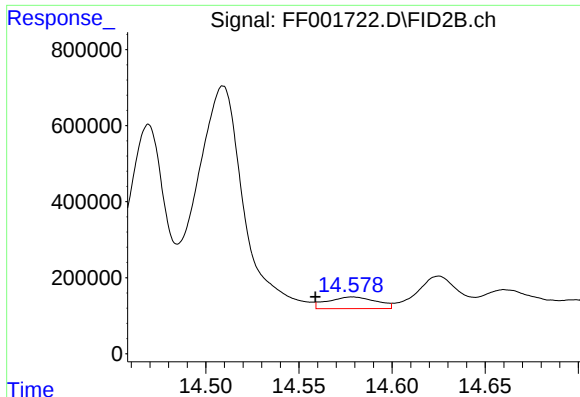


#10 N-TETRACOSANE

R.T.: 14.579 min
Delta R.T.: 0.020 min
Response: 551190
Conc: 1.74 ug/ml

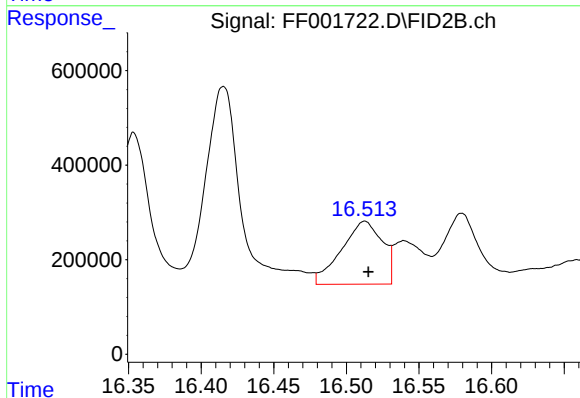


#11 N-OCTACOSANE

R.T.: 16.513 min
Delta R.T.: -0.002 min
Response: 2612956
Conc: 8.12 ug/ml

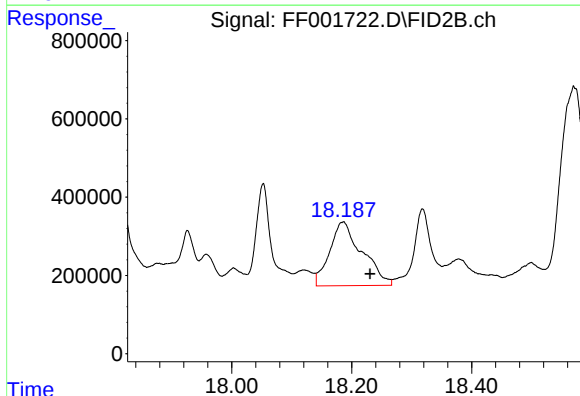


#12 N-DOTRIACONTANE

R.T.: 18.185 min
Delta R.T.: -0.045 min
Response: 6130946
Conc: 18.79 ug/ml

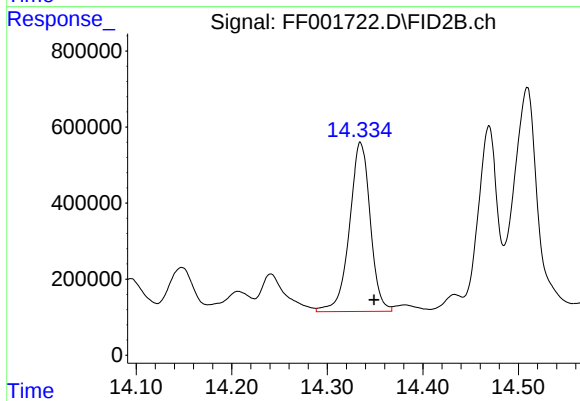


#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.335 min
Delta R.T.: -0.014 min
Response: 6731000
Conc: 16.70 ug/ml

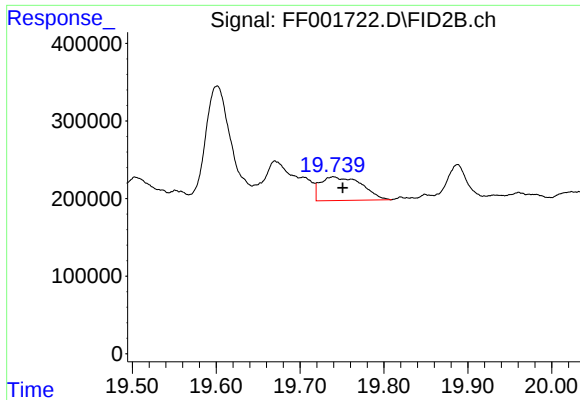

#14 N-HEXATRIACONTANE

R.T.: 19.739 min
Delta R.T.: -0.012 min
Response: 1037594
Conc: 3.52 ug/ml

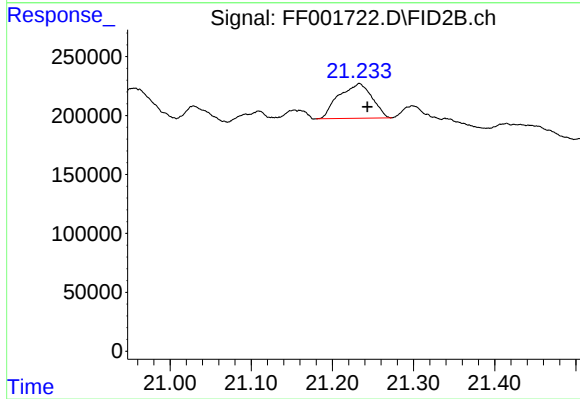

#15 N-TETRACONTANE

R.T.: 21.233 min
Delta R.T.: -0.010 min
Response: 835734
Conc: 3.47 ug/ml