

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080718\
 Data File : FF001729.D
 Signal(s) : FID2B.ch
 Acq On : 07 Aug 2018 20:37
 Operator : AJ\SJ
 Sample : J4305-06
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Aug 08 00:59:33 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF080418.M
 Quant Title :
 QLast Update : Mon Aug 06 12:04:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
13) S	TETRACOSANE-d50 (SURR...	14.330	6553031	16.256 ug/ml
Target Compounds				
6)	N-TETRADECANE	7.966	2891521	9.266 ug/ml
7)	N-HEXADECANE	9.494	348869	1.108 ug/ml
8)	N-OCTADECANE	10.928	275571	0.874 ug/ml
9)	N-EICOSANE	12.293	252684	0.801 ug/ml
10)	N-TETRACOSANE	14.527	796161	2.506 ug/ml
11)	N-OCTACOSANE	16.535	1108049	3.443 ug/ml
12)	N-DOTRIACONTANE	18.207	1213953	3.721 ug/ml
15)	N-TETRACONTANE	21.301	1593927	6.620 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080718\
Data File : FF001729.D
Signal(s) : FID2B.ch
Acq On : 07 Aug 2018 20:37
Operator : AJ\SJ
Sample : J4305-06
Misc :
ALS Vial : 66 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 08 00:59:33 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF080418.M
Quant Title :
QLast Update : Mon Aug 06 12:04:39 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

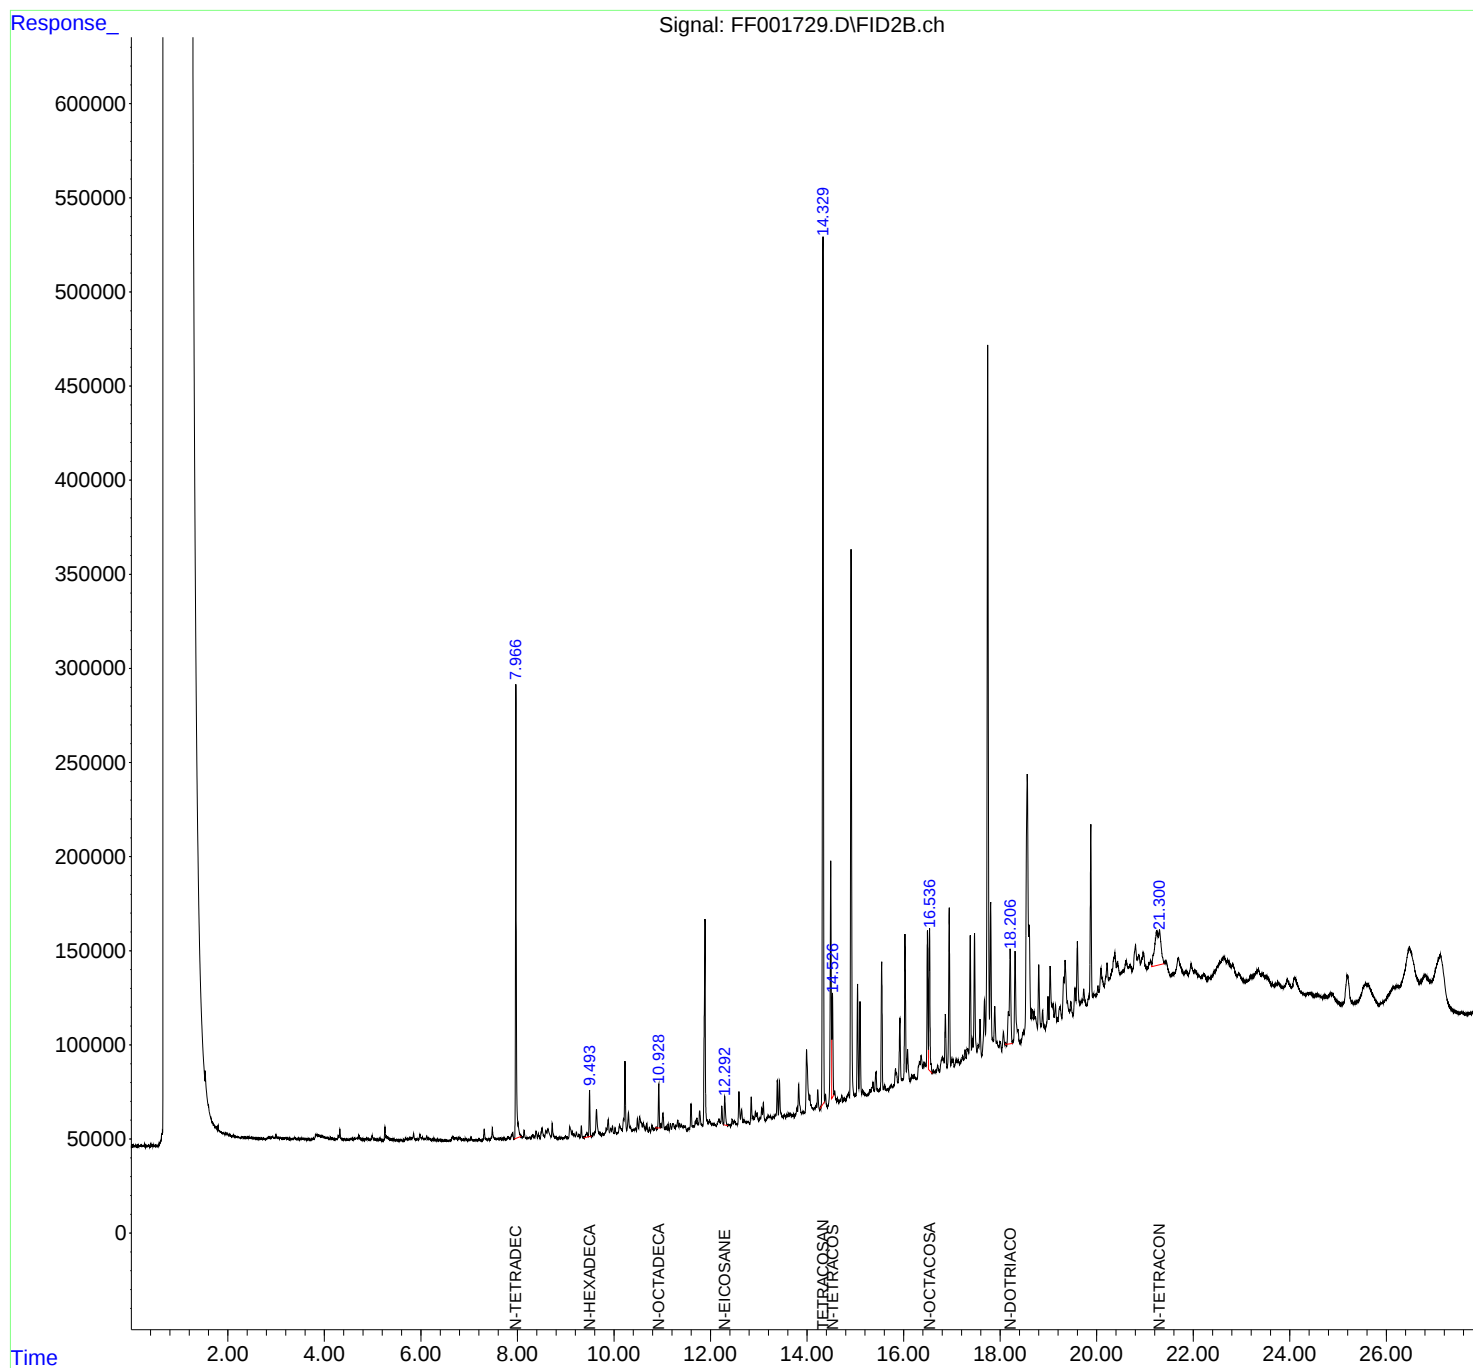

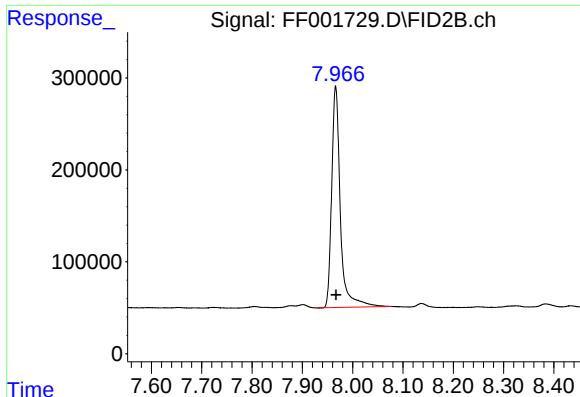


#6 N-TETRADECANE

R.T.: 7.966 min
Delta R.T.: 0.000 min
Response: 2891521
Conc: 9.27 ug/ml

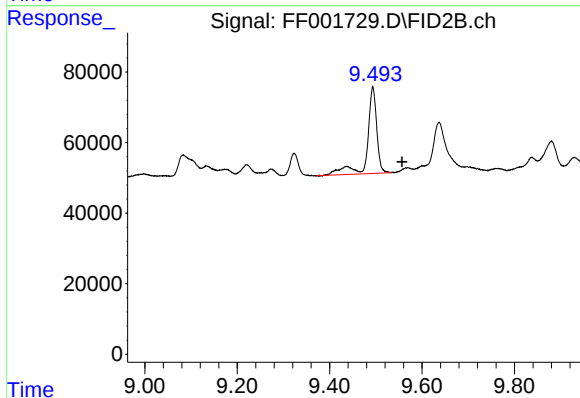


#7 N-HEXADECANE

R.T.: 9.494 min
Delta R.T.: -0.064 min
Response: 348869
Conc: 1.11 ug/ml

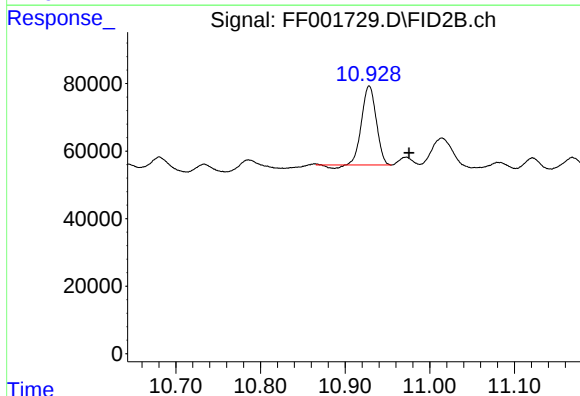


#8 N-OCTADECANE

R.T.: 10.928 min
Delta R.T.: -0.047 min
Response: 275571
Conc: 0.87 ug/ml

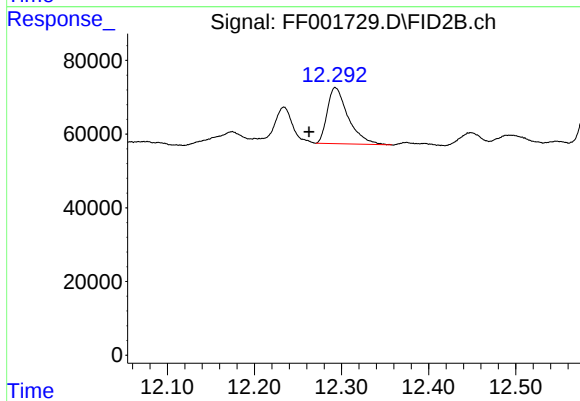


#9 N-EICOSANE

R.T.: 12.293 min
Delta R.T.: 0.031 min
Response: 252684
Conc: 0.80 ug/ml

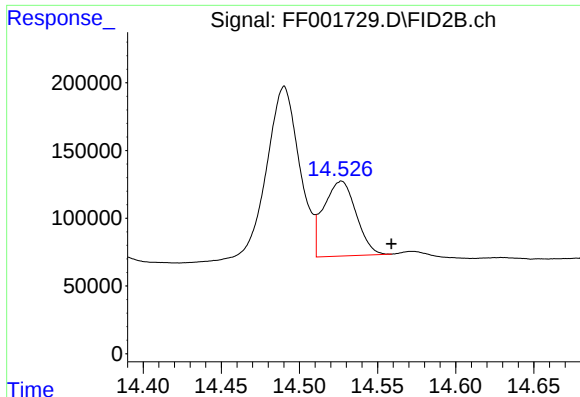


#10 N-TETRACOSANE

R.T.: 14.527 min
Delta R.T.: -0.032 min
Response: 796161
Conc: 2.51 ug/ml

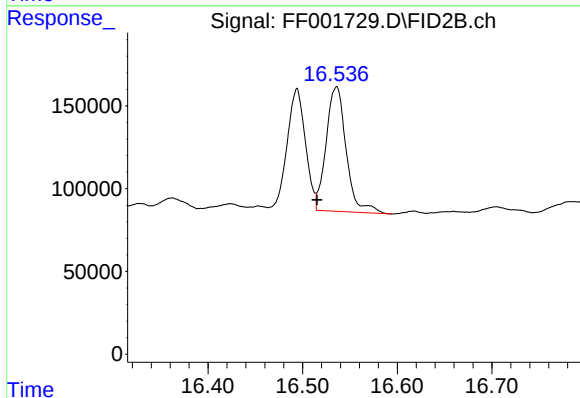


#11 N-OCTACOSANE

R.T.: 16.535 min
Delta R.T.: 0.020 min
Response: 1108049
Conc: 3.44 ug/ml

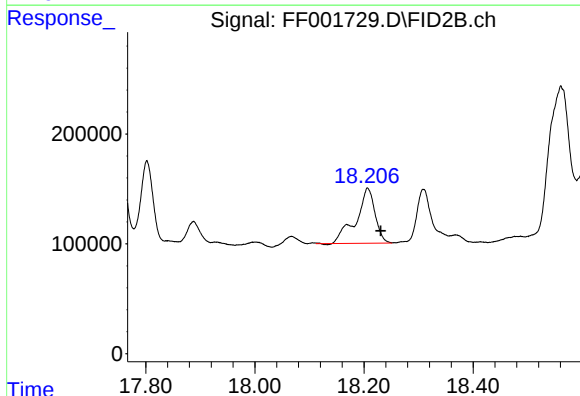


#12 N-DOTRIACONTANE

R.T.: 18.207 min
Delta R.T.: -0.024 min
Response: 1213953
Conc: 3.72 ug/ml

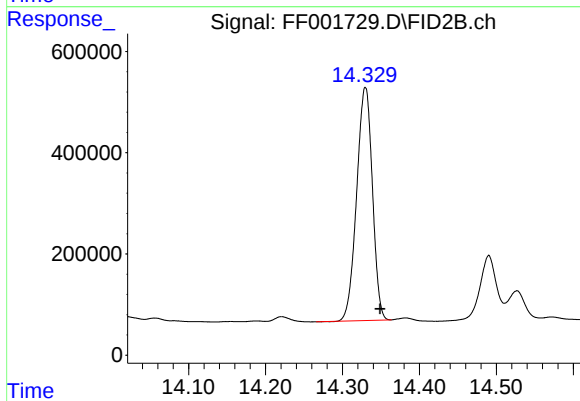

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.330 min
Delta R.T.: -0.019 min
Response: 6553031
Conc: 16.26 ug/ml

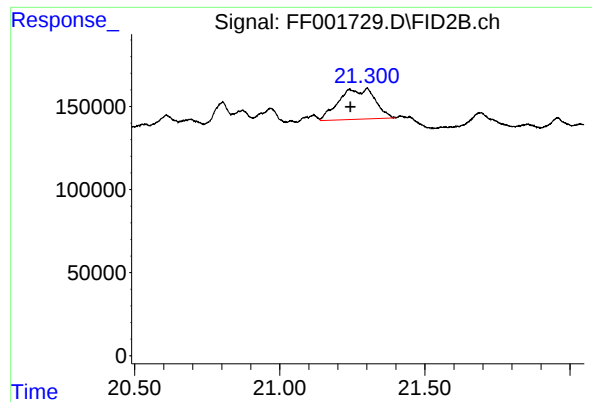

#15 N-TETRACONTANE

R.T.: 21.301 min
Delta R.T.: 0.058 min
Response: 1593927
Conc: 6.62 ug/ml