

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080718\
Data File : FF001733.D
Signal(s) : FID2B.ch
Acq On : 07 Aug 2018 23:02
Operator : AJ\SJ
Sample : J4348-04
Misc :
ALS Vial : 70 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 08 01:00:32 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF080418.M
Quant Title :
QLast Update : Mon Aug 06 12:04:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.327	4919546	12.204 ug/ml
Target Compounds			
6) N-TETRADECANE	7.968	770394	2.469 ug/ml
9) N-EICOSANE	12.288	754847	2.393 ug/ml
10) N-TETRACOSANE	14.489	2860373	9.004 ug/ml
11) N-OCTACOSANE	16.533	157298	0.489 ug/ml
12) N-DOTRIACONTANE	18.204	803913	2.464 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF080718\
Data File : FF001733.D
Signal(s) : FID2B.ch
Acq On : 07 Aug 2018 23:02
Operator : AJ\SJ
Sample : J4348-04
Misc :
ALS Vial : 70 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 08 01:00:32 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\C44-FF080418.M
Quant Title :
QLast Update : Mon Aug 06 12:04:39 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

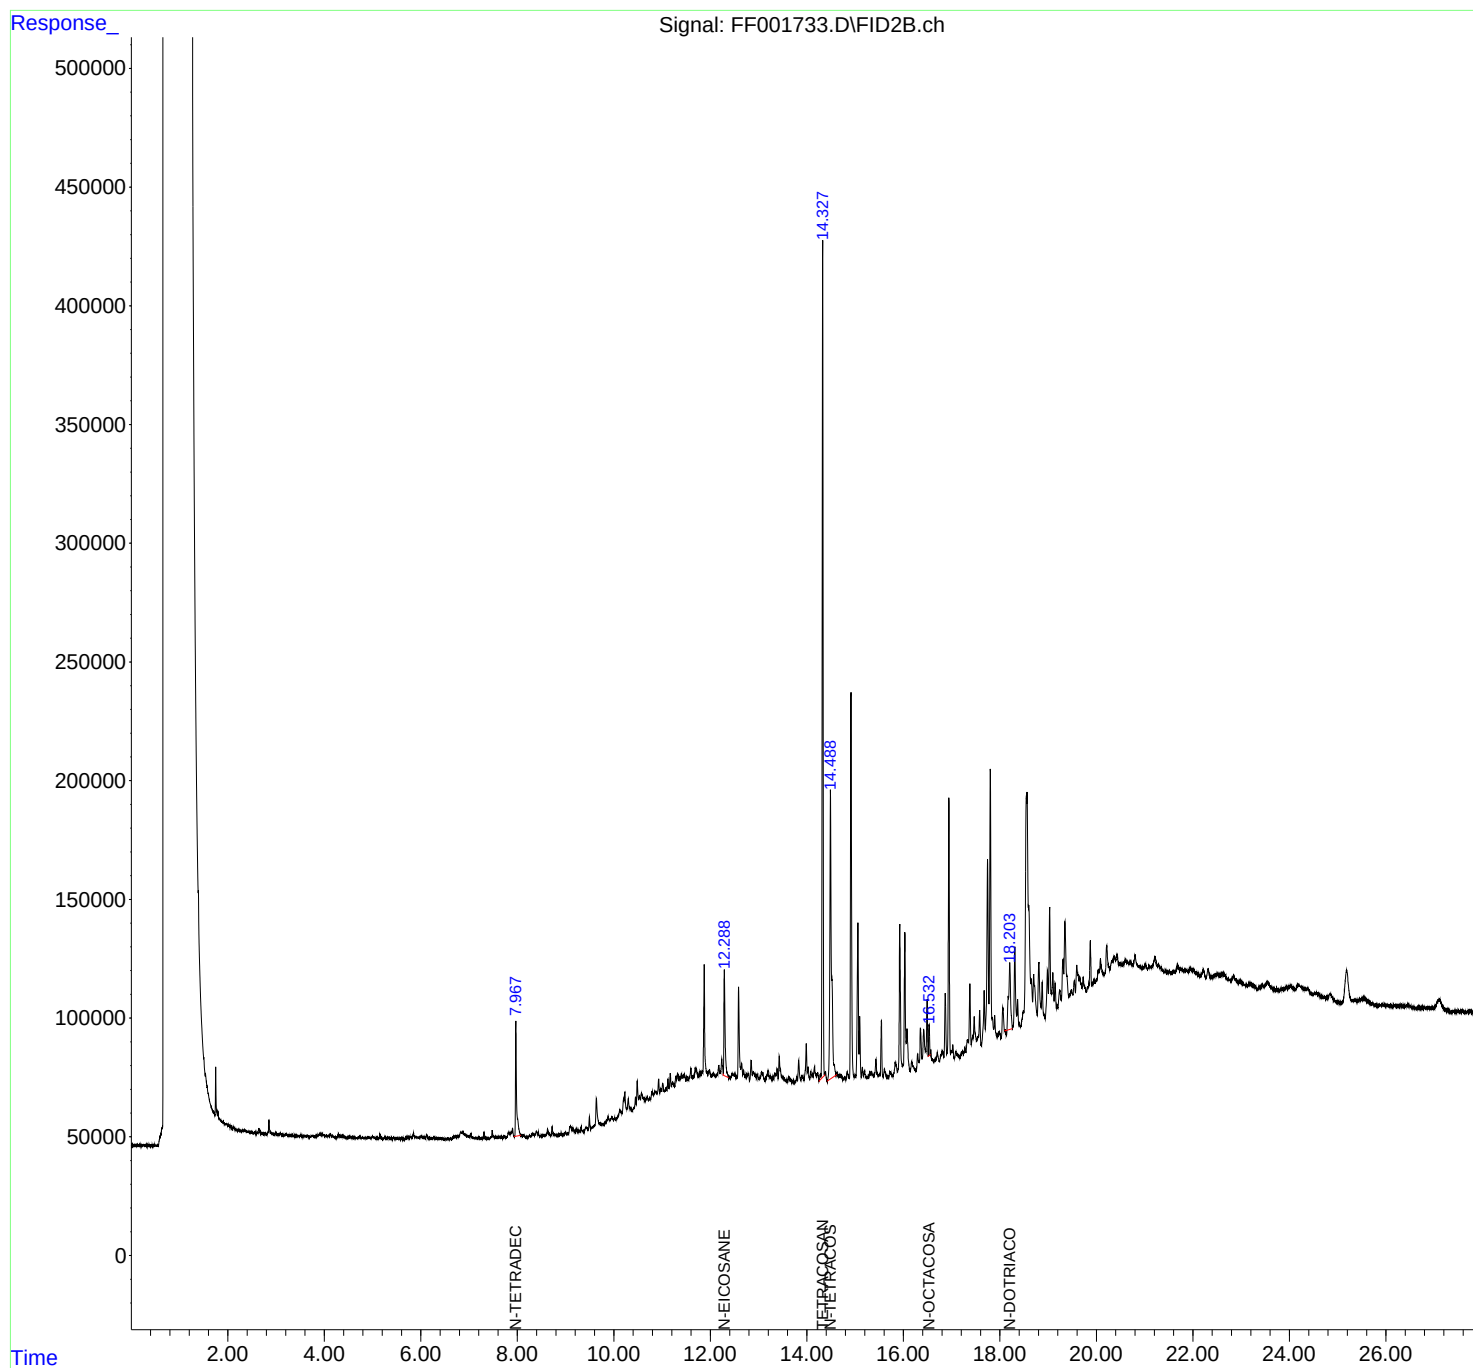

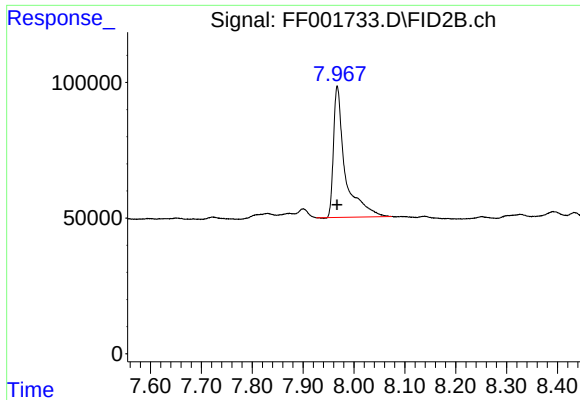


#6 N-TETRADECANE

R.T.: 7.968 min
Delta R.T.: 0.000 min
Response: 770394
Conc: 2.47 ug/ml

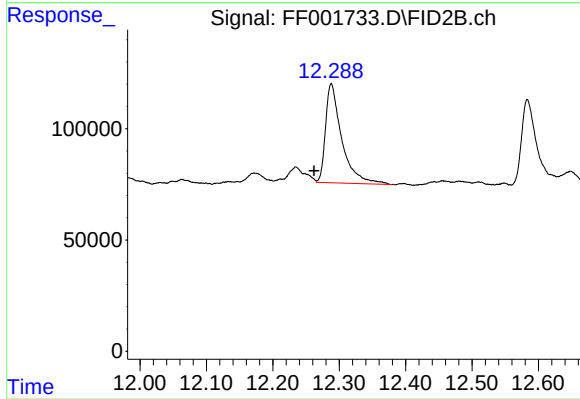


#9 N-EICOSANE

R.T.: 12.288 min
Delta R.T.: 0.026 min
Response: 754847
Conc: 2.39 ug/ml

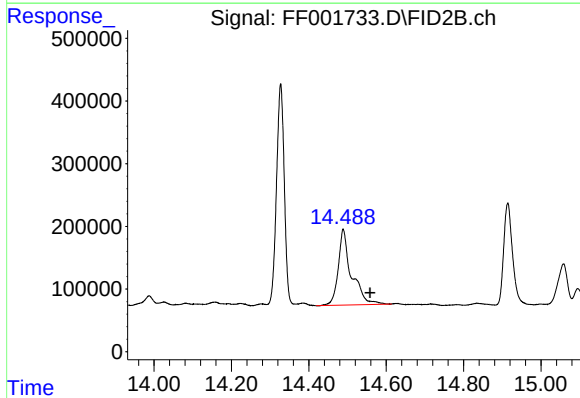


#10 N-TETRACOSANE

R.T.: 14.489 min
Delta R.T.: -0.070 min
Response: 2860373
Conc: 9.00 ug/ml

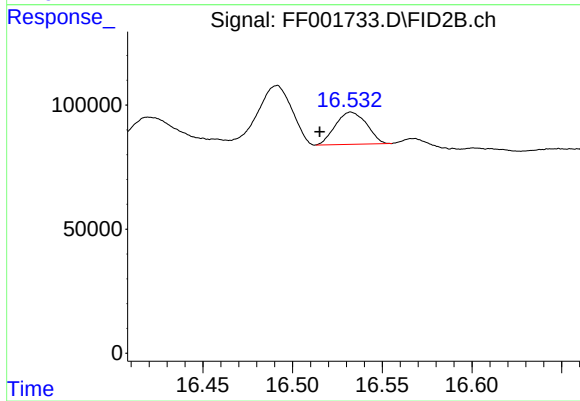


#11 N-OCTACOSANE

R.T.: 16.533 min
Delta R.T.: 0.018 min
Response: 157298
Conc: 0.49 ug/ml

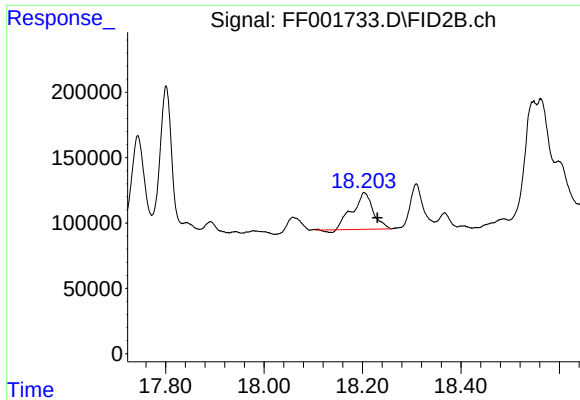

#12 N-DOTRIACONTANE

R.T.: 18.204 min
Delta R.T.: -0.027 min
Response: 803913
Conc: 2.46 ug/ml

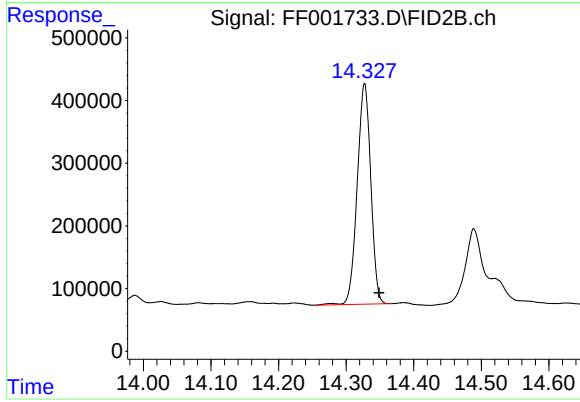

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.327 min
Delta R.T.: -0.022 min
Response: 4919546
Conc: 12.20 ug/ml