

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG080819\
 Data File : FG005579.D
 Signal(s) : FID1A.ch
 Acq On : 08 Aug 2019 12:00
 Operator : DD\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 08 14:45:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080819.M
 Quant Title :
 QLast Update : Thu Aug 08 14:43:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
11) N-HEXACOSANE	15.984	56278	0.406 ug/ml
12) N-OCTACOSANE	16.937	288910	2.093 ug/ml
13) N-TRIACONTANE	17.825	287476	2.143 ug/ml
14) N-DOTRIACONTANE	18.662	194917	1.543 ug/ml
15) N-TETRATRIACONTANE	19.450	27584	0.235 ug/ml
16) N-HEXATRIACONTANE	20.215	234762	2.018 ug/ml
17) N-OCTATRIACONTANE	20.957	69975	0.684 ug/ml
18) N-TETRACONTANE	21.916	279840	2.537 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG080819\
Data File : FG005579.D
Signal(s) : FID1A.ch
Acq On : 08 Aug 2019 12:00
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampled :

Integration File: autoint1.e
Quant Time: Aug 08 14:45:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080819.M
Quant Title :
QLast Update : Thu Aug 08 14:43:49 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

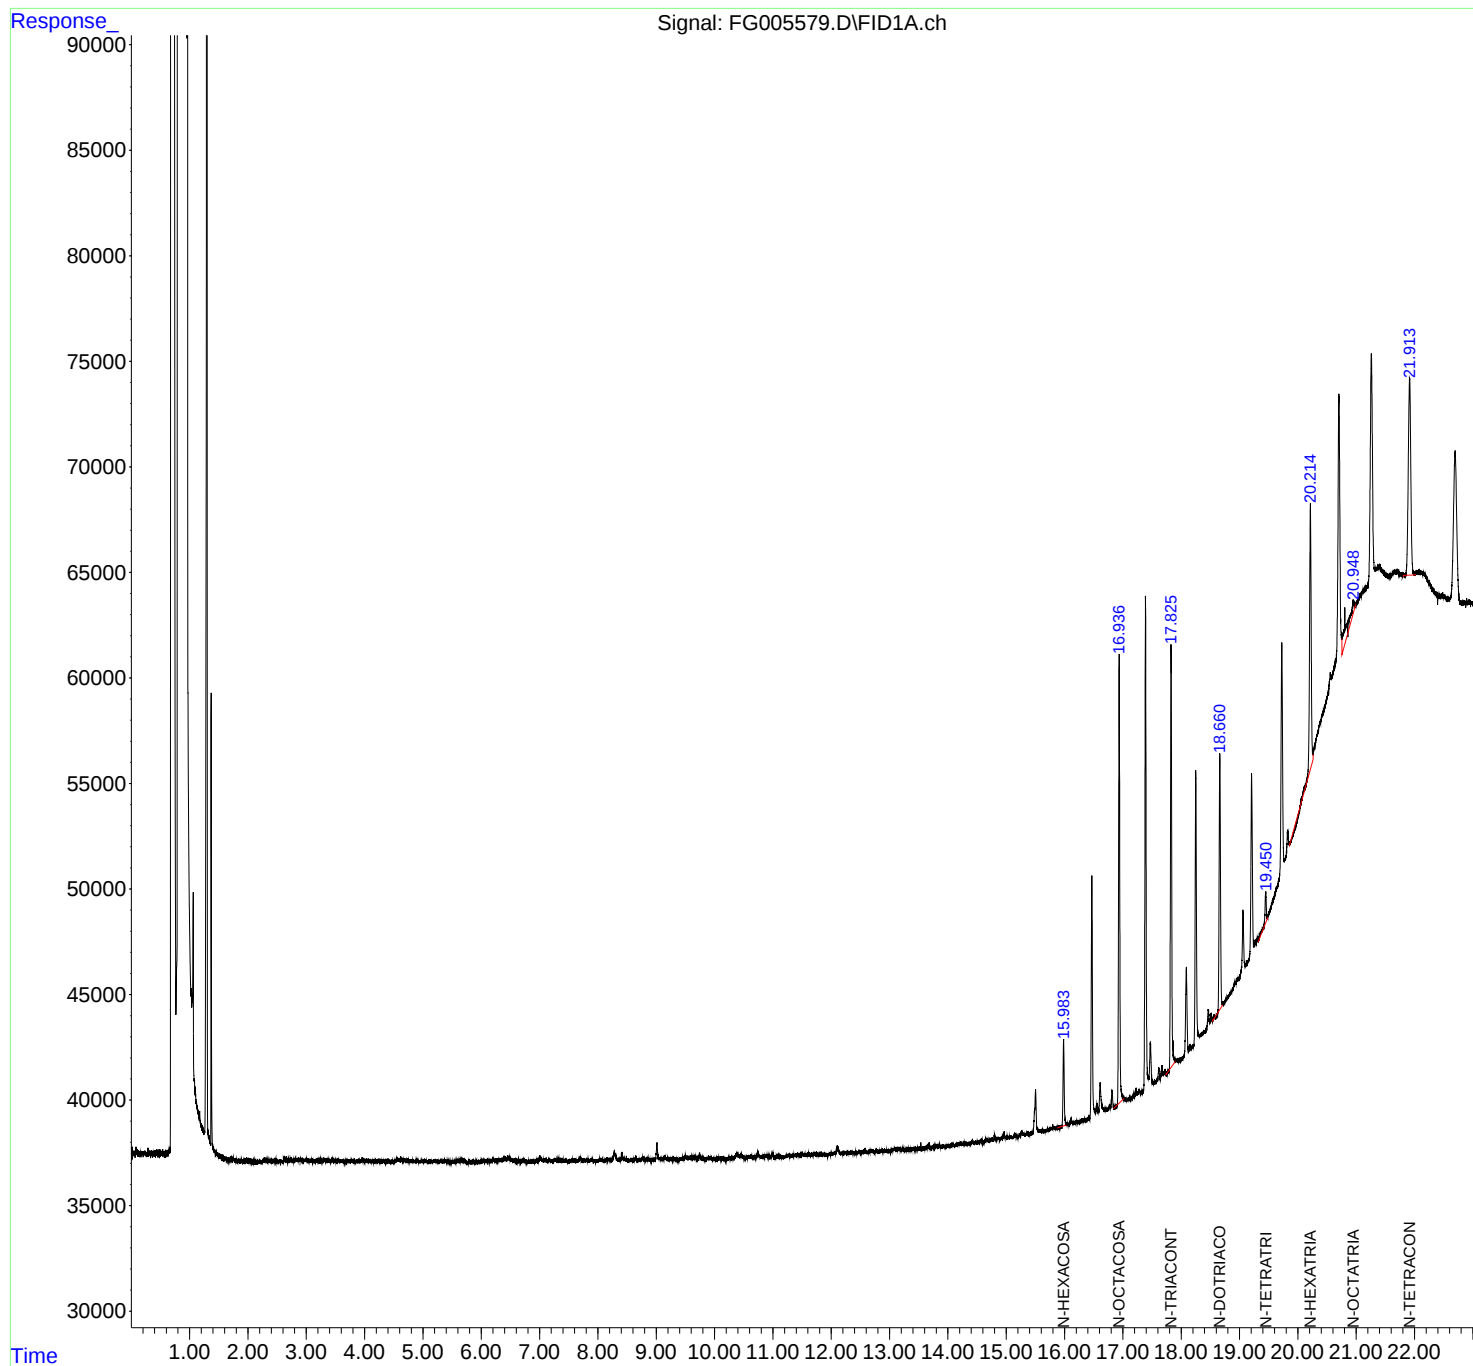


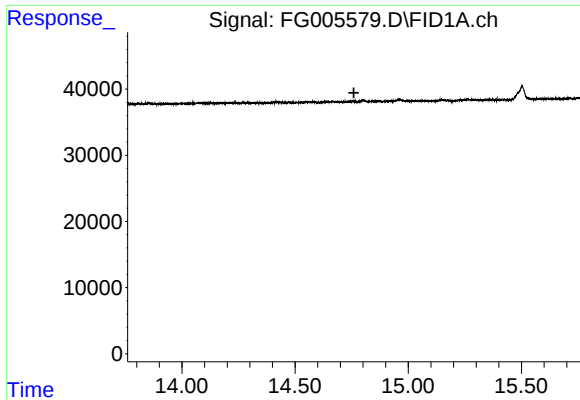

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.760 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

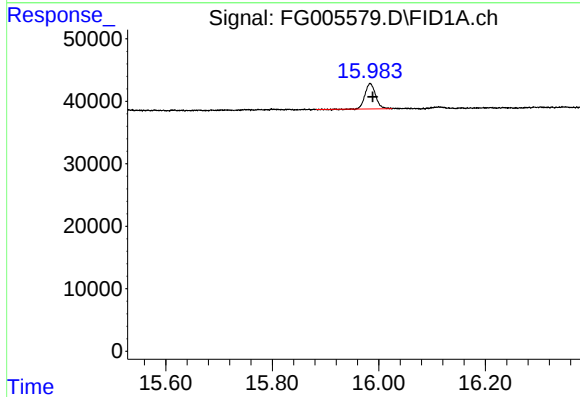


#11 N-HEXACOSANE

R.T.: 15.984 min
Delta R.T.: -0.004 min
Response: 56278
Conc: 0.41 ug/ml

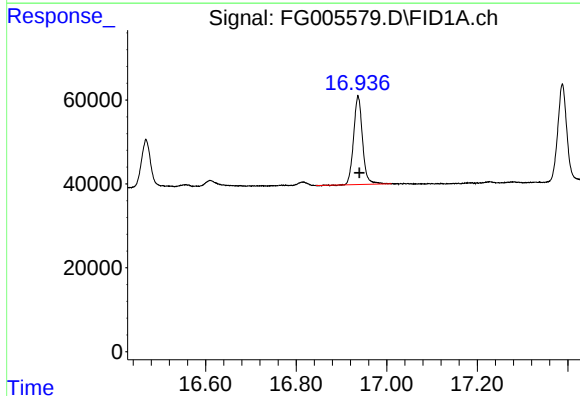


#12 N-OCTACOSANE

R.T.: 16.937 min
Delta R.T.: -0.003 min
Response: 288910
Conc: 2.09 ug/ml

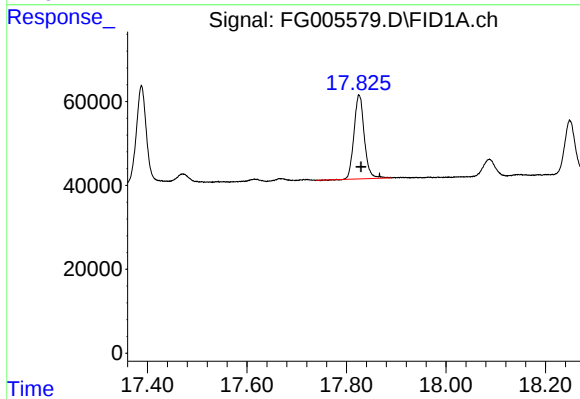

#13 N-TRIACONTANE


R.T.: 17.825 min
Delta R.T.: -0.004 min
Response: 287476
Conc: 2.14 ug/ml

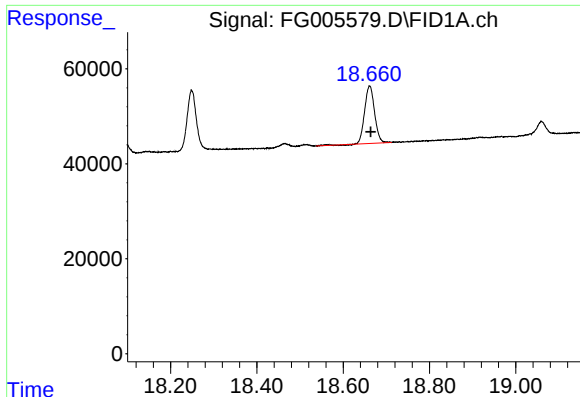

#14 N-DOTRIACONTANE


R.T.: 18.662 min
Delta R.T.: -0.002 min
Response: 194917
Conc: 1.54 ug/ml

Instrument :
FID_G
ClientSampleId :

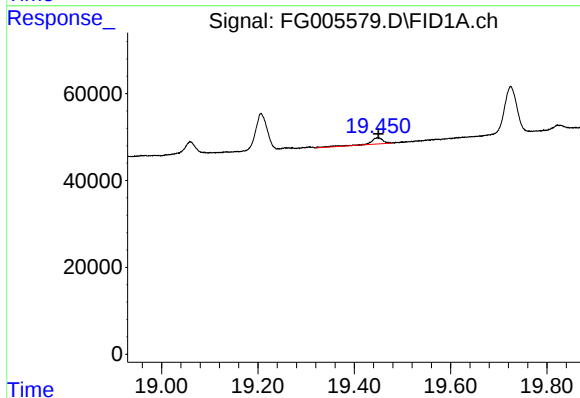


#15 N-TETRATRIACONTANE

R.T.: 19.450 min
Delta R.T.: 0.000 min
Response: 27584
Conc: 0.23 ug/ml

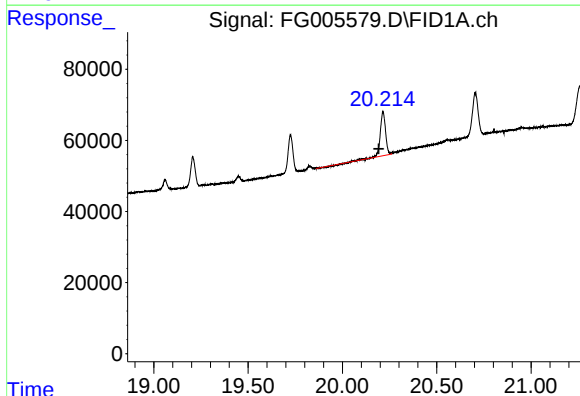


#16 N-HEXATRIACONTANE

R.T.: 20.215 min
Delta R.T.: 0.021 min
Response: 234762
Conc: 2.02 ug/ml

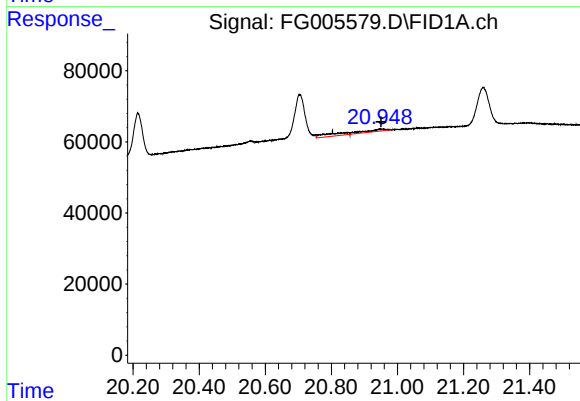

#17 N-OCTATRIACONTANE

R.T.: 20.957 min
Delta R.T.: 0.006 min
Response: 69975
Conc: 0.68 ug/ml

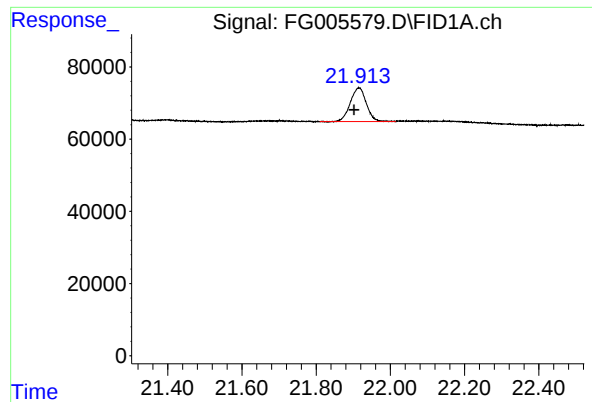

#18 N-TETRACONTANE

R.T.: 21.916 min
Delta R.T.: 0.014 min
Response: 279840
Conc: 2.54 ug/ml

Instrument :
FID_G
ClientSampleId :