

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG080823\
Data File : FG012619.D
Signal(s) : FID1A.ch
Acq On : 08 Aug 2023 11:18
Operator : YP\AJ
Sample : PB154659BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB154659BL

Integration File: autoint1.e
Quant Time: Aug 09 02:17:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080223.M
Quant Title :
QLast Update : Wed Aug 02 18:57:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.079	2193938	19.612 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG080823\
Data File : FG012619.D
Signal(s) : FID1A.ch
Acq On : 08 Aug 2023 11:18
Operator : YP\AJ
Sample : PB154659BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB154659BL

Integration File: autoint1.e
Quant Time: Aug 09 02:17:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080223.M
Quant Title :
QLast Update : Wed Aug 02 18:57:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

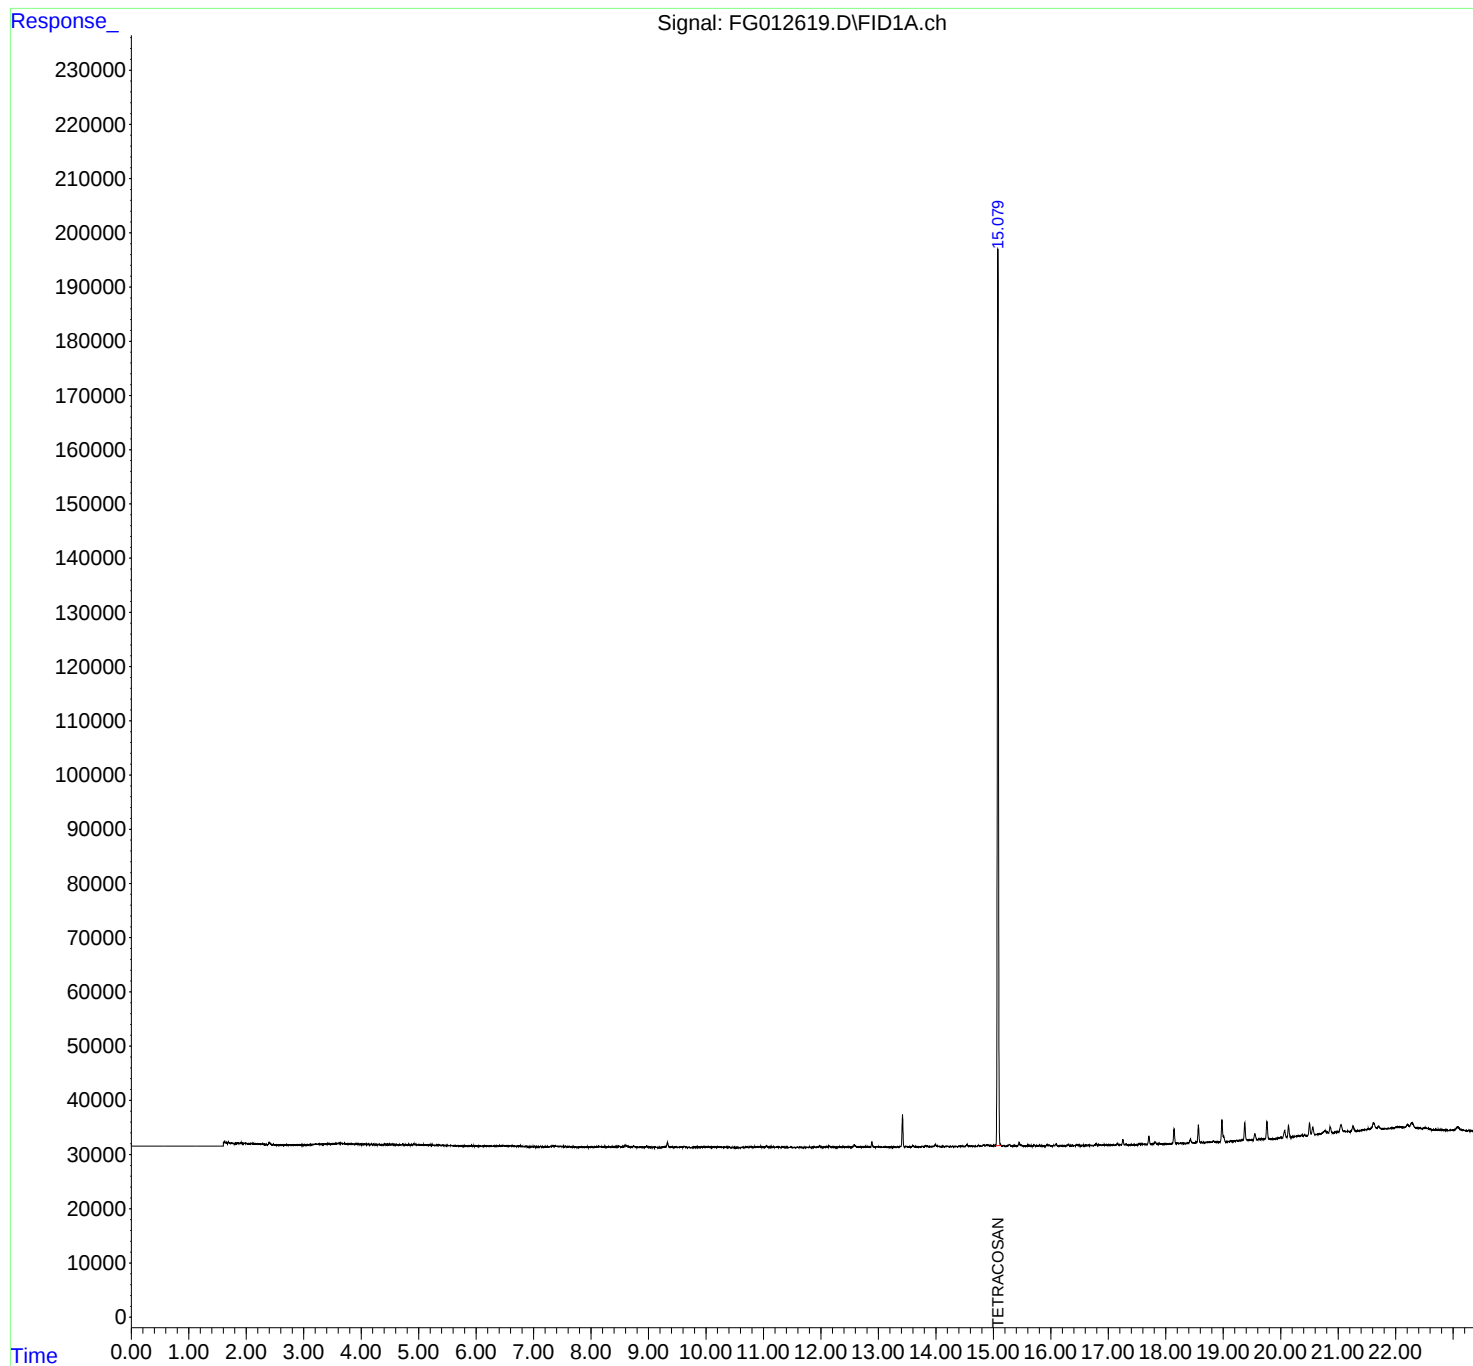

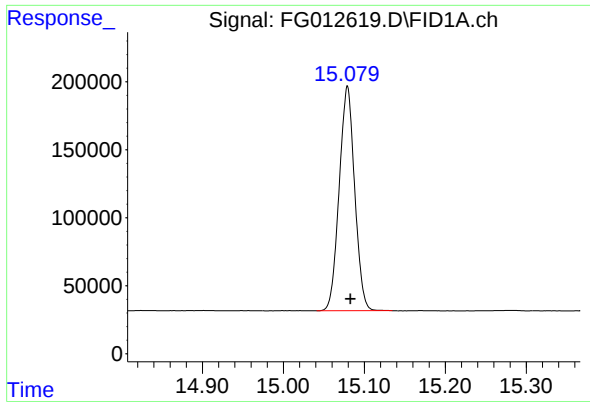

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.079 min
Delta R.T.: -0.004 min
Response: 2193938
Conc: 19.61 ug/ml

Instrument :
FID_G
ClientSampleId :
PB154659BL