

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG080823\
Data File : FG012632.D
Signal(s) : FID1A.ch
Acq On : 08 Aug 2023 17:46
Operator : YP\AJ
Sample : PB154660BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB154660BL

Integration File: autoint1.e
Quant Time: Aug 09 02:24:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080223.M
Quant Title :
QLast Update : Wed Aug 02 18:57:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.078	2189728	19.575 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG080823\
Data File : FG012632.D
Signal(s) : FID1A.ch
Acq On : 08 Aug 2023 17:46
Operator : YP\AJ
Sample : PB154660BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB154660BL

Integration File: autoint1.e
Quant Time: Aug 09 02:24:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080223.M
Quant Title :
QLast Update : Wed Aug 02 18:57:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

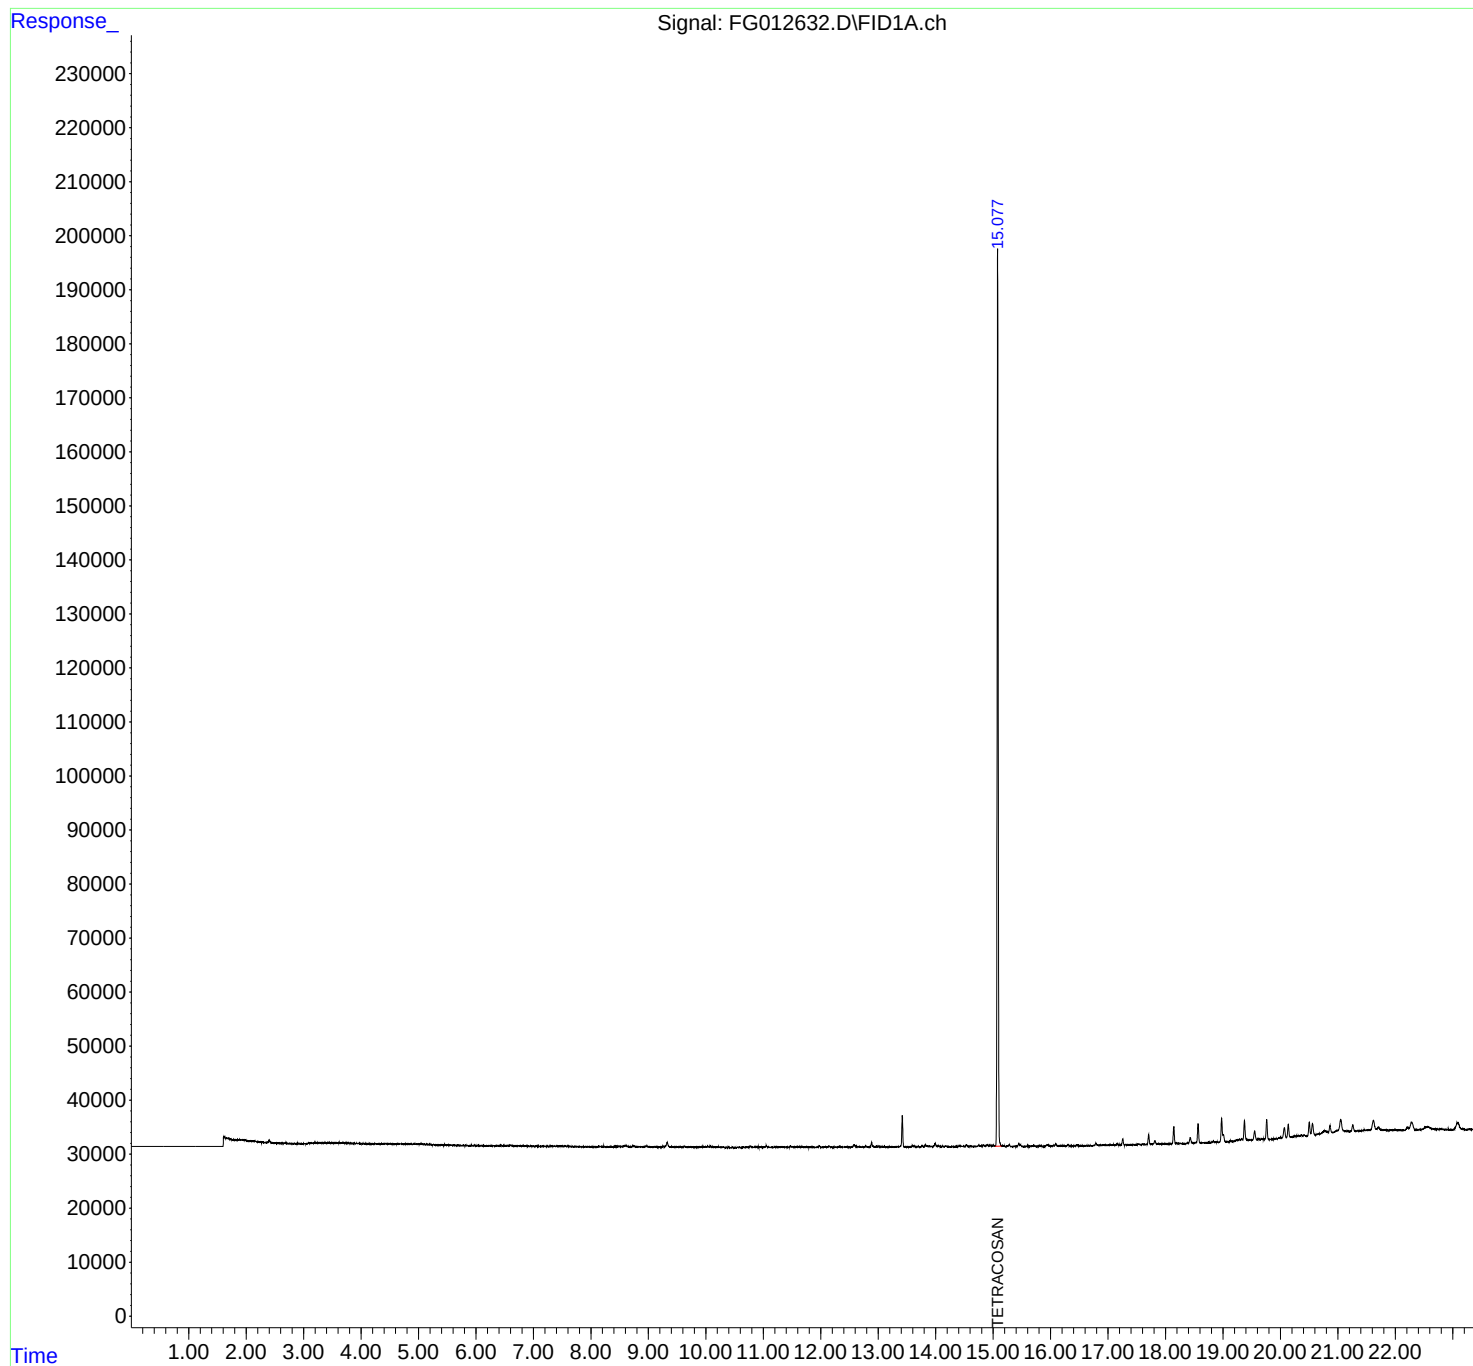

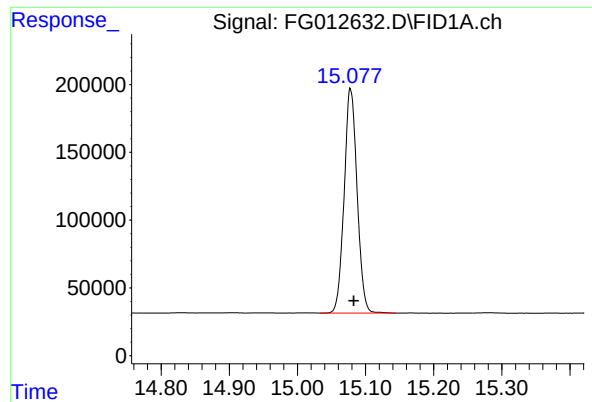

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.078 min
Delta R.T.: -0.005 min
Response: 2189728
Conc: 19.57 ug/ml

Instrument :

FID_G

ClientSampleId :

PB154660BL