

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG080923\
Data File : FG012651.D
Signal(s) : FID1A.ch
Acq On : 09 Aug 2023 18:16
Operator : YP\AJ
Sample : PB154670BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 09 23:57:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080223.M
Quant Title :
QLast Update : Wed Aug 02 18:57:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.079	2267035	20.266 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.978	46940	0.418 ug/ml
15) N-TETRATRIACONTANE	19.764	46764	0.494 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG080923\
Data File : FG012651.D
Signal(s) : FID1A.ch
Acq On : 09 Aug 2023 18:16
Operator : YP\AJ
Sample : PB154670BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 09 23:57:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080223.M
Quant Title :
QLast Update : Wed Aug 02 18:57:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

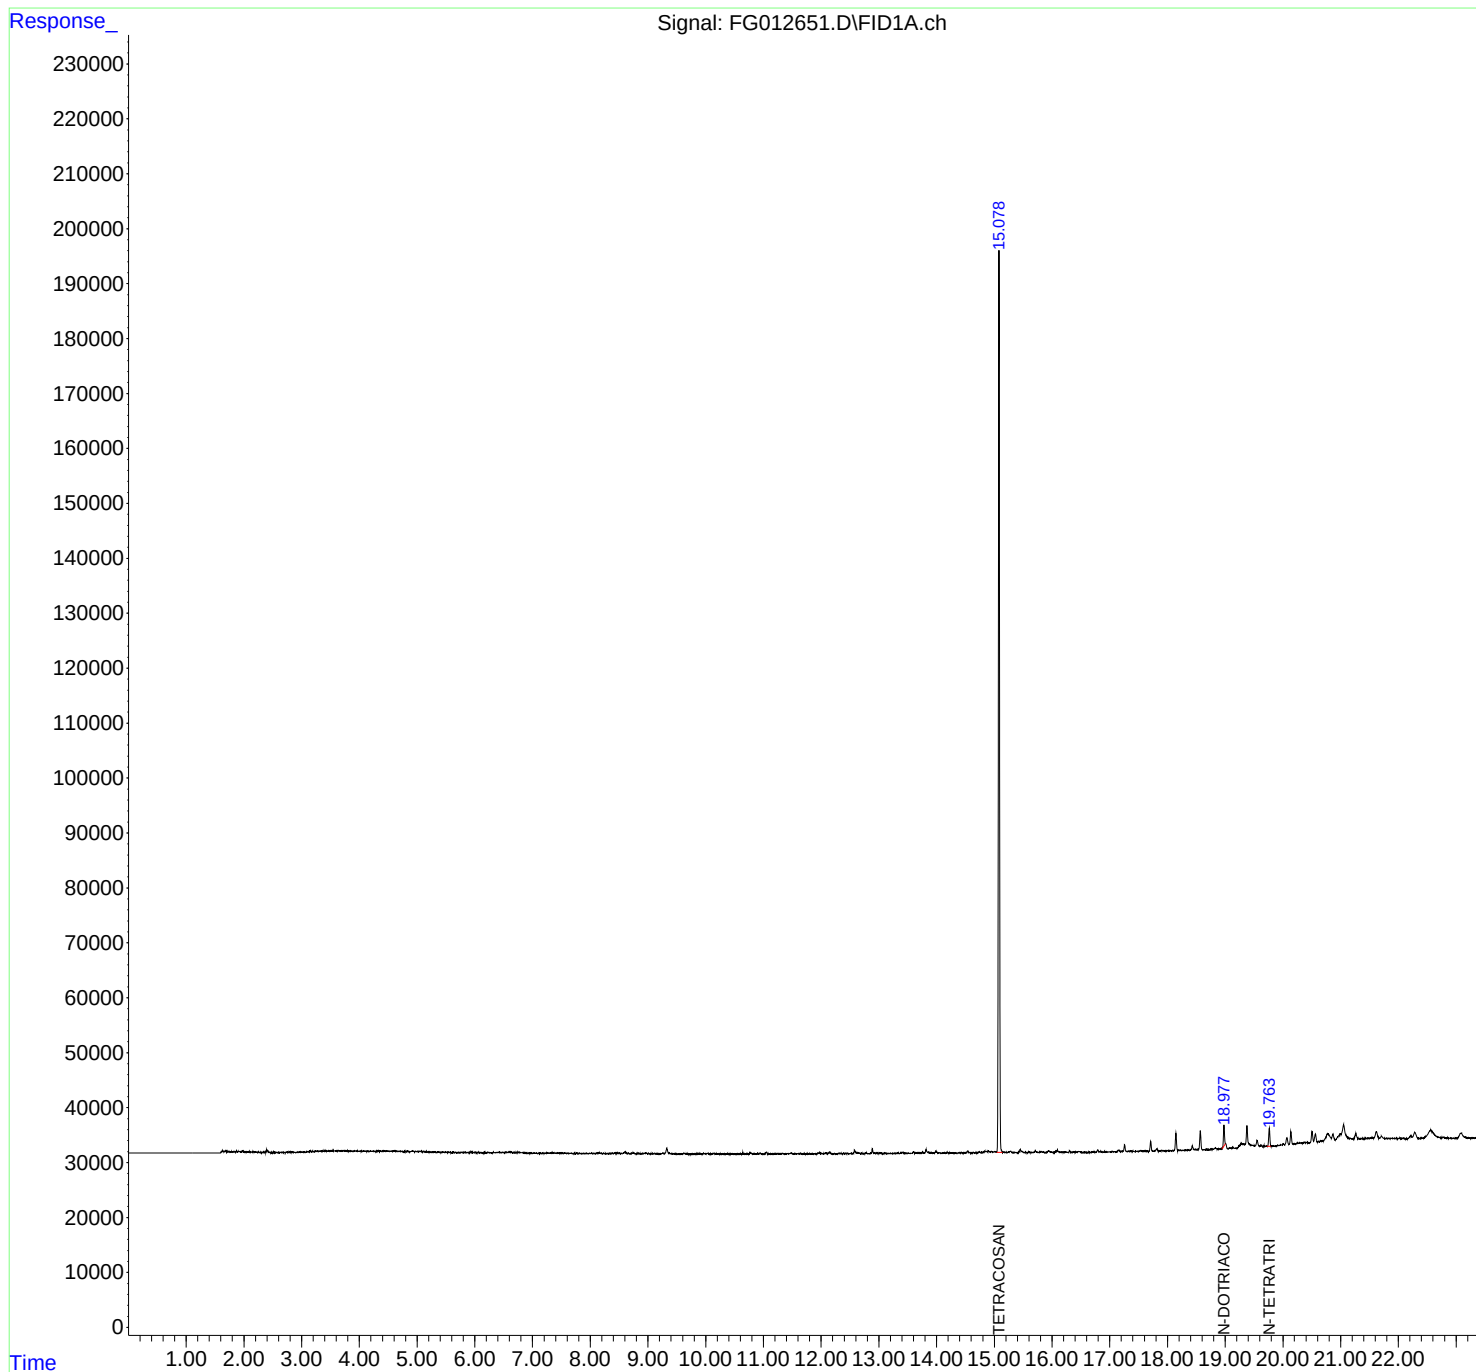


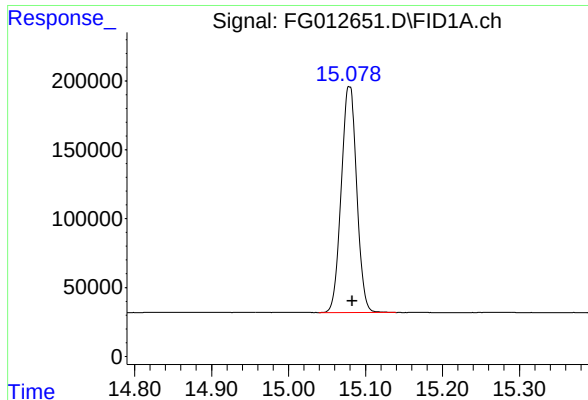

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.079 min
Delta R.T.: -0.003 min
Response: 2267035
Conc: 20.27 ug/ml

Instrument :
FID_G
ClientSampleId :

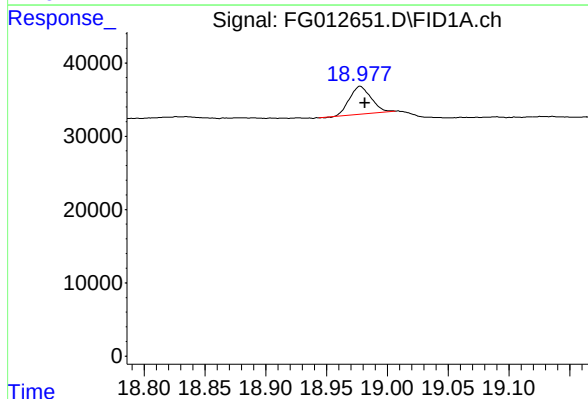

#14 N-DOTRIACONTANE

R.T.: 18.978 min
Delta R.T.: -0.004 min
Response: 46940
Conc: 0.42 ug/ml

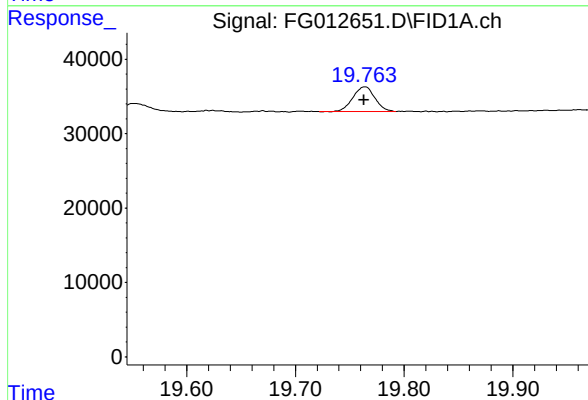

#15 N-TETRATRIACONTANE

R.T.: 19.764 min
Delta R.T.: 0.000 min
Response: 46764
Conc: 0.49 ug/ml