

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081018\
 Data File : FG002047.D
 Signal(s) : FID1A.ch
 Acq On : 10 Aug 2018 17:15
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 11 02:19:55 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG073018.M
 Quant Title :
 QLast Update : Mon Jul 30 13:56:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.461	2157246	17.114 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.523	91612	0.671 ug/ml
14) N-DOTRIACONTANE	18.357	289255	2.336 ug/ml
15) N-TETRATRIACONTANE	19.142	179198	1.648 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081018\
Data File : FG002047.D
Signal(s) : FID1A.ch
Acq On : 10 Aug 2018 17:15
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 11 02:19:55 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG073018.M
Quant Title :
QLast Update : Mon Jul 30 13:56:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

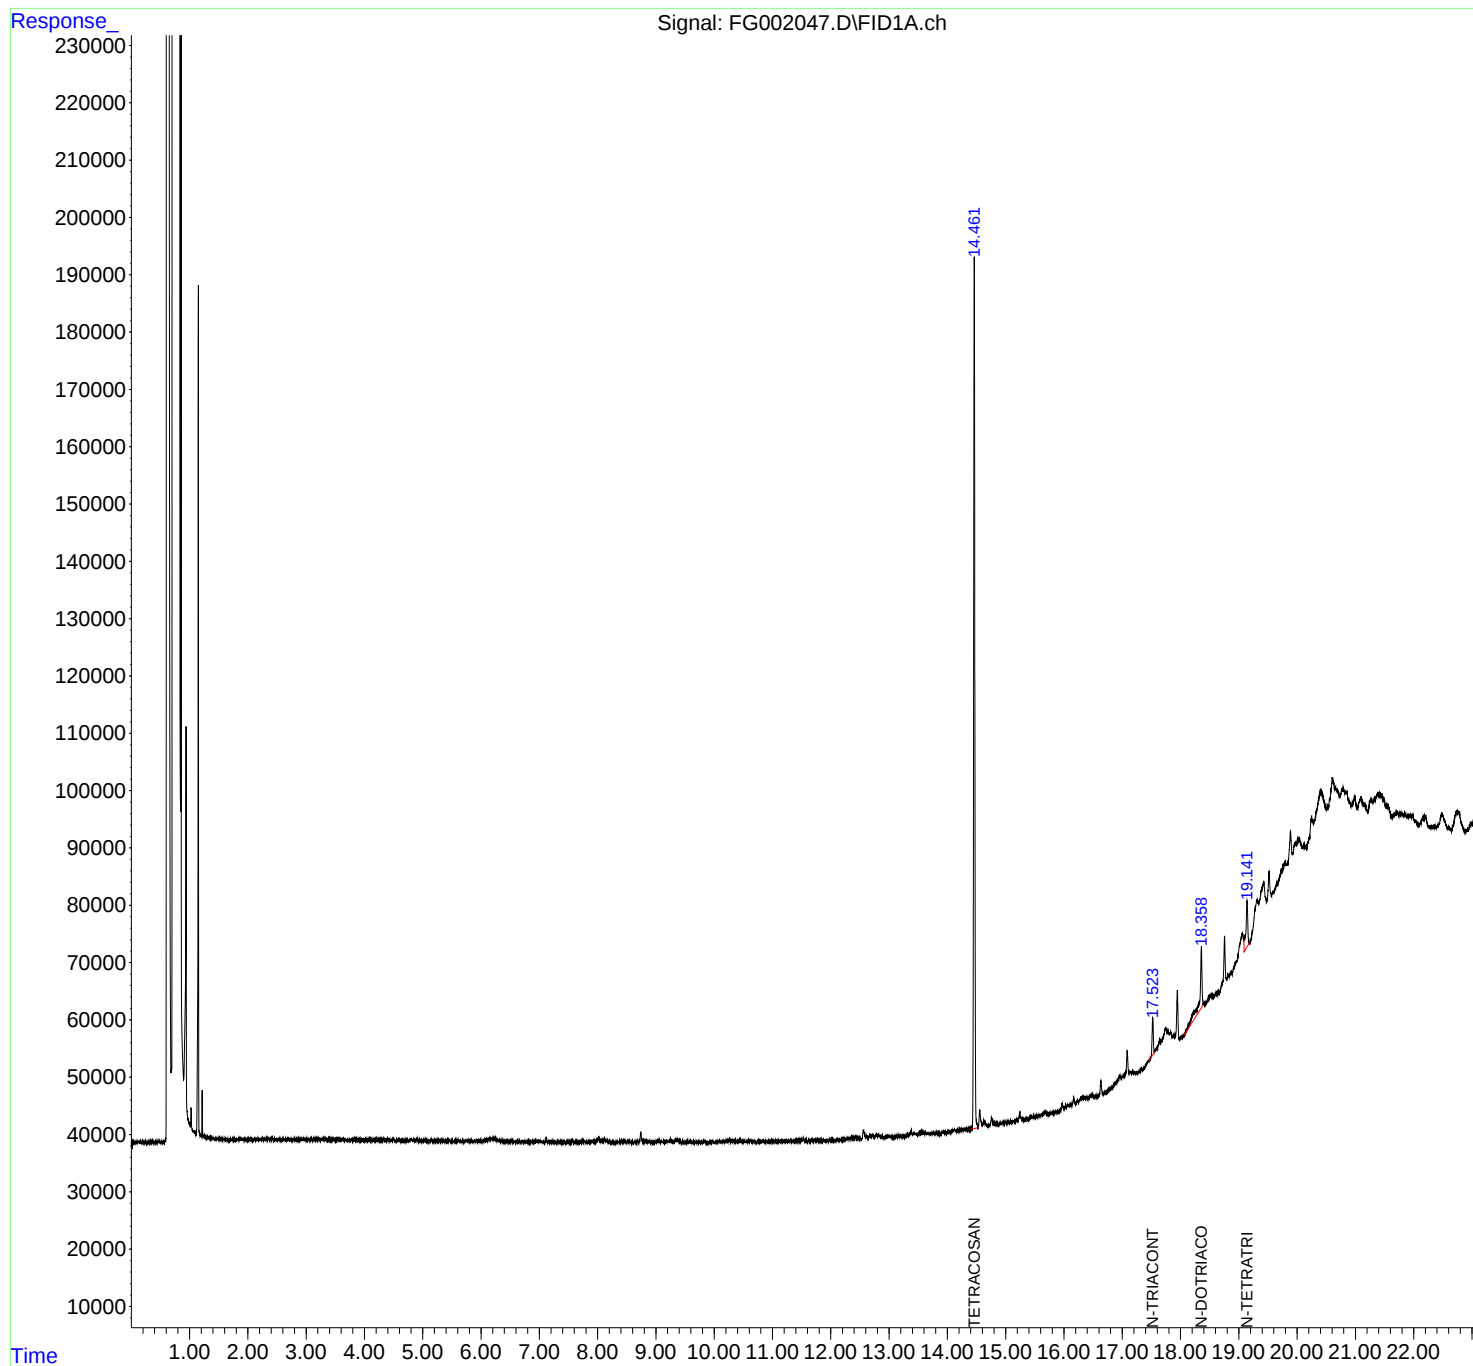


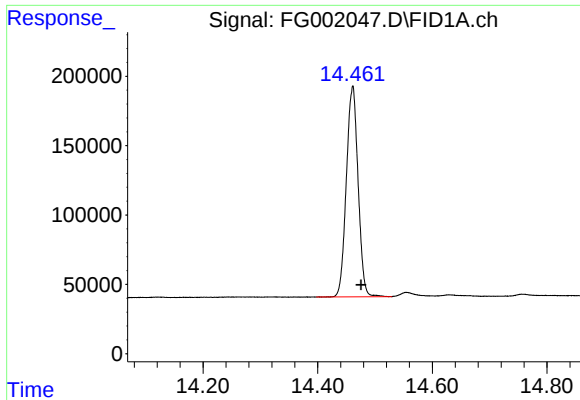

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.461 min
Delta R.T.: -0.014 min
Response: 2157246
Conc: 17.11 ug/ml

Instrument :
FID_G
ClientSampleId :

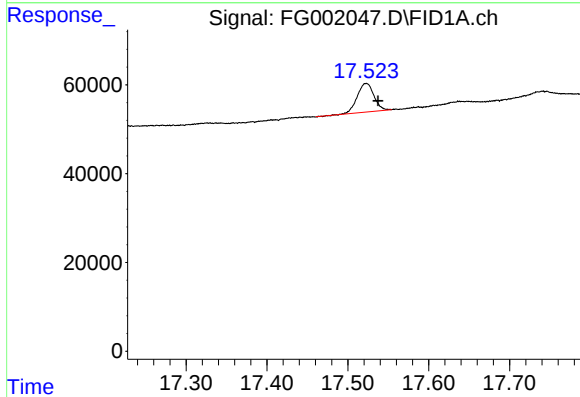


#13 N-TRIACONTANE

R.T.: 17.523 min
Delta R.T.: -0.015 min
Response: 91612
Conc: 0.67 ug/ml

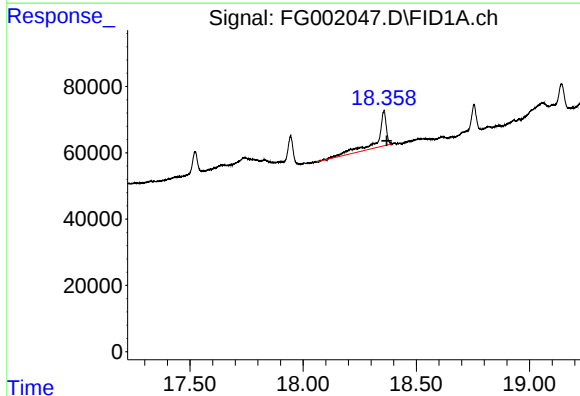

#14 N-DOTRIACONTANE

R.T.: 18.357 min
Delta R.T.: -0.013 min
Response: 289255
Conc: 2.34 ug/ml

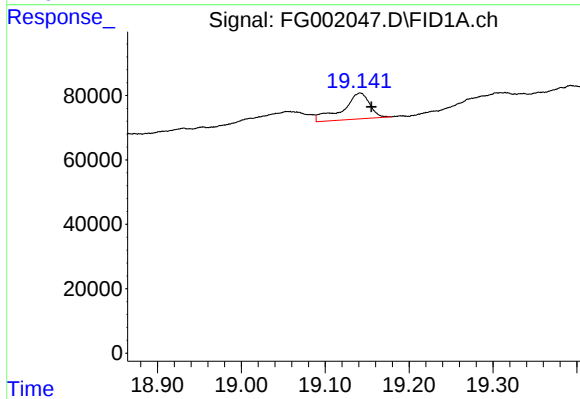

#15 N-TETRATRIACONTANE

R.T.: 19.142 min
Delta R.T.: -0.013 min
Response: 179198
Conc: 1.65 ug/ml