

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081018\
 Data File : FG002056.D
 Signal(s) : FID1A.ch
 Acq On : 10 Aug 2018 21:56
 Operator : AJ\SJ
 Sample : J4409-11 5X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 11 02:21:38 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG073018.M
 Quant Title :
 QLast Update : Mon Jul 30 13:56:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.459	374619	2.972 ug/ml
Target Compounds			
4) N-TETRADECANE	8.079	72516	0.477 ug/ml
7) N-EICOSANE	12.410	444266	2.944 ug/ml
10) N-TETRACOSANE	14.632	301753	2.105 ug/ml
12) N-OCTACOSANE	16.635	140209	1.005 ug/ml
13) N-TRIACONTANE	17.523	196101	1.436 ug/ml
14) N-DOTRIACONTANE	18.353	326961	2.640 ug/ml
15) N-TETRATRIACONTANE	19.141	262184	2.411 ug/ml
16) N-HEXATRIACONTANE	19.879	198000	2.061 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081018\
Data File : FG002056.D
Signal(s) : FID1A.ch
Acq On : 10 Aug 2018 21:56
Operator : AJ\SJ
Sample : J4409-11 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 11 02:21:38 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG073018.M
Quant Title :
QLast Update : Mon Jul 30 13:56:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

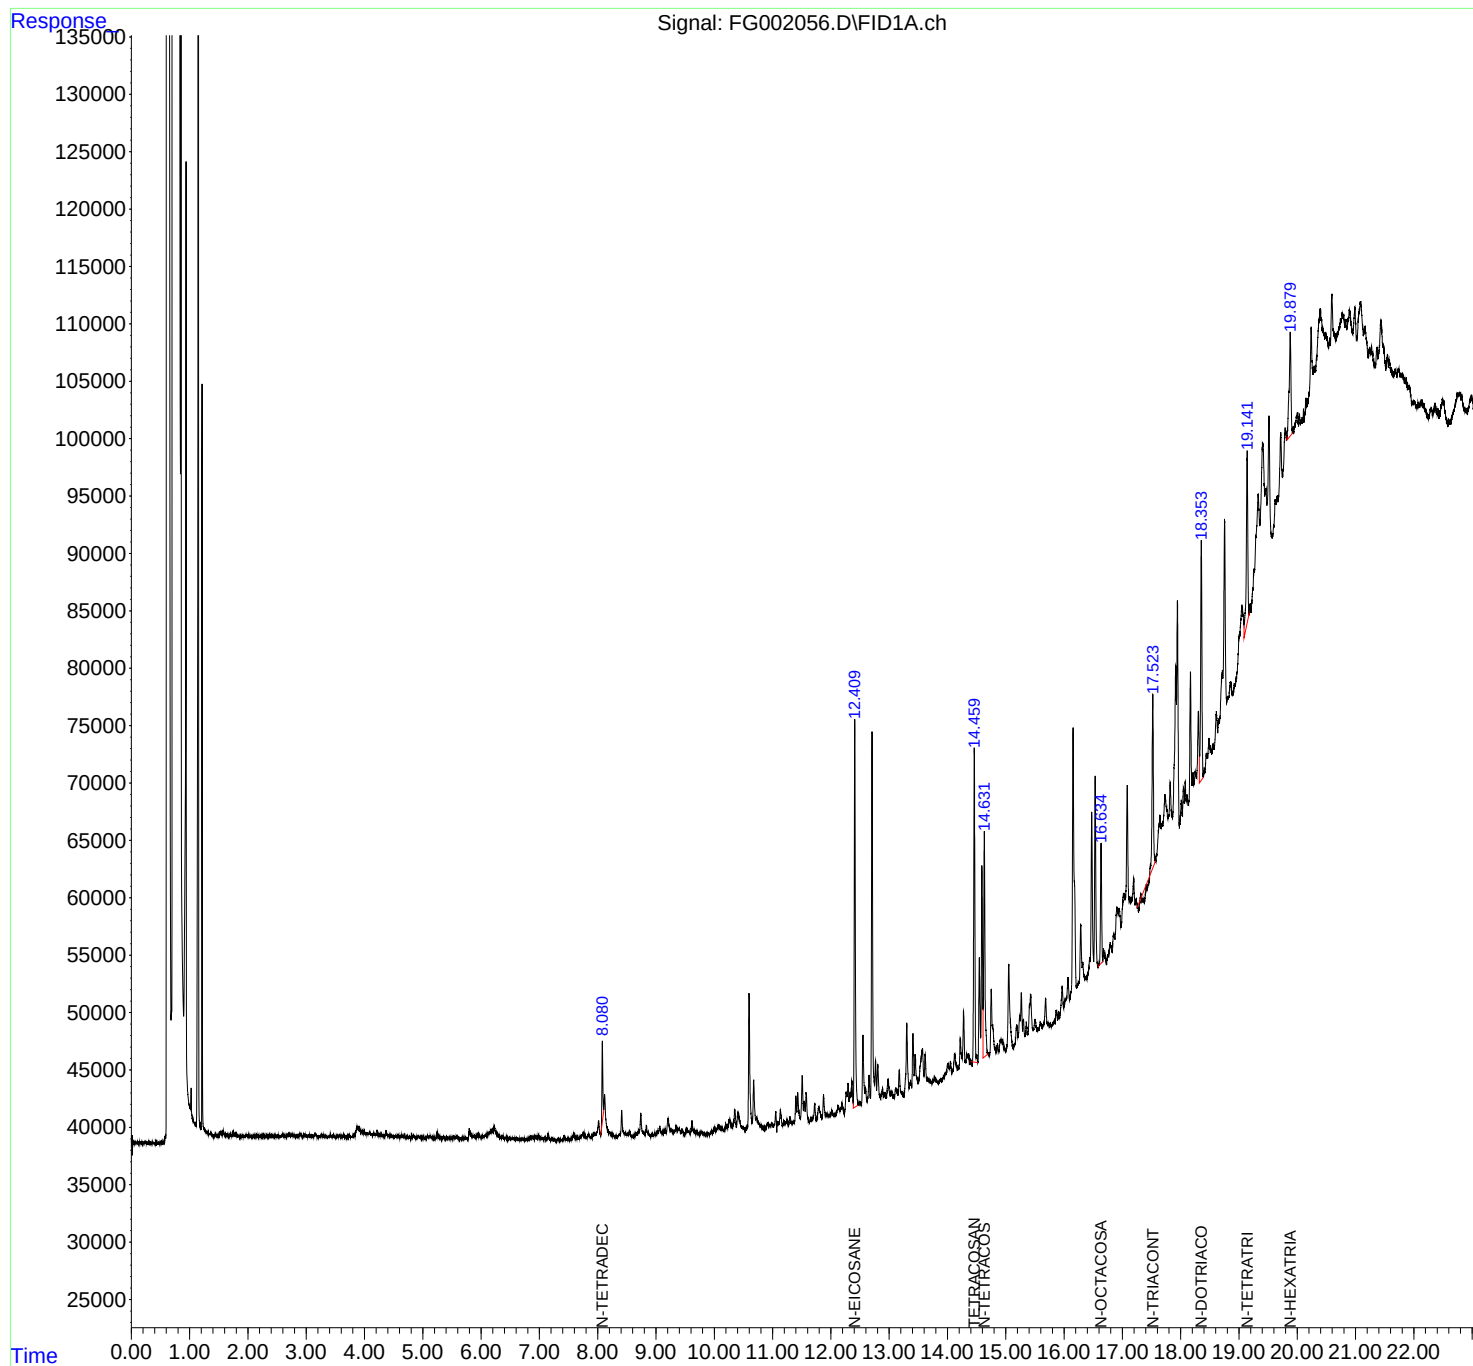


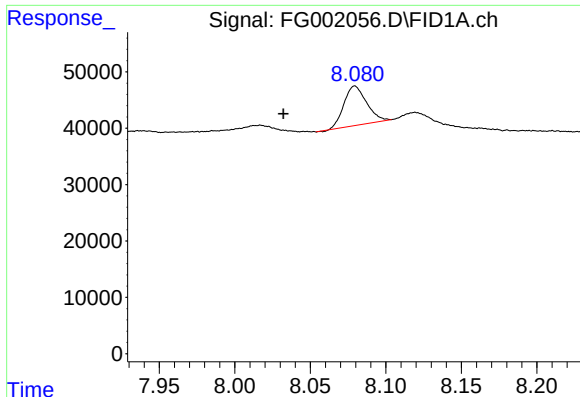

#4 N-TETRADECANE


R.T.: 8.079 min
Delta R.T.: 0.047 min
Response: 72516
Conc: 0.48 ug/ml

Instrument :
FID_G
ClientSampleId :

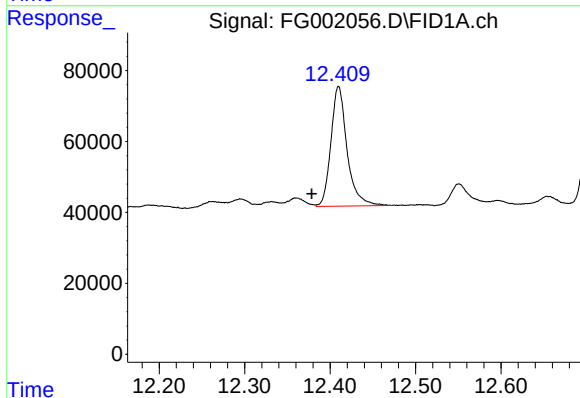


#7 N-EICOSANE

R.T.: 12.410 min
Delta R.T.: 0.032 min
Response: 444266
Conc: 2.94 ug/ml

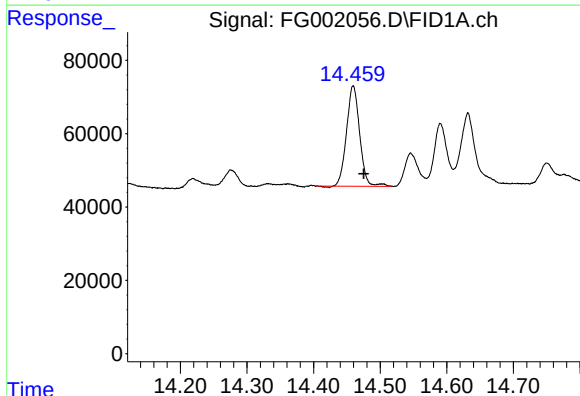


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.459 min
Delta R.T.: -0.016 min
Response: 374619
Conc: 2.97 ug/ml

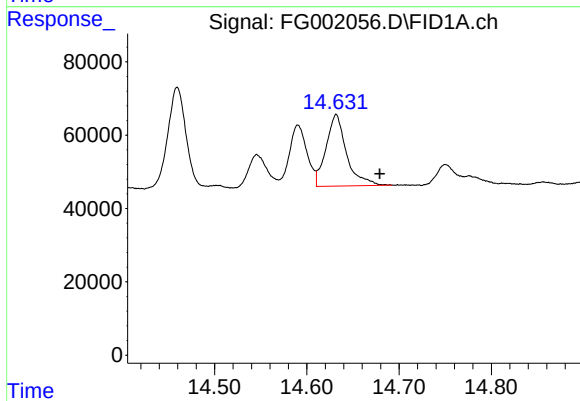

#10 N-TETRACOSANE


R.T.: 14.632 min
Delta R.T.: -0.047 min
Response: 301753
Conc: 2.10 ug/ml

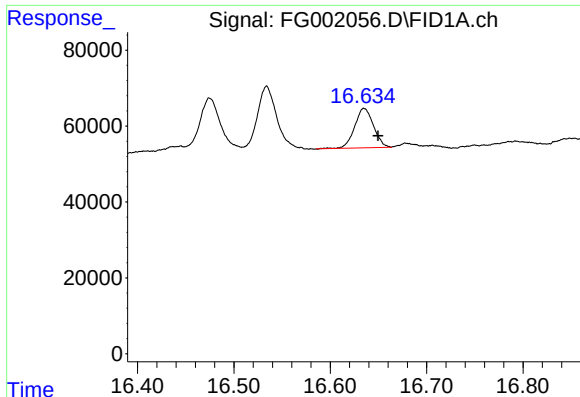

#12 N-OCTACOSANE


R.T.: 16.635 min
Delta R.T.: -0.014 min
Response: 140209
Conc: 1.00 ug/ml

Instrument :
FID_G
ClientSampleId :

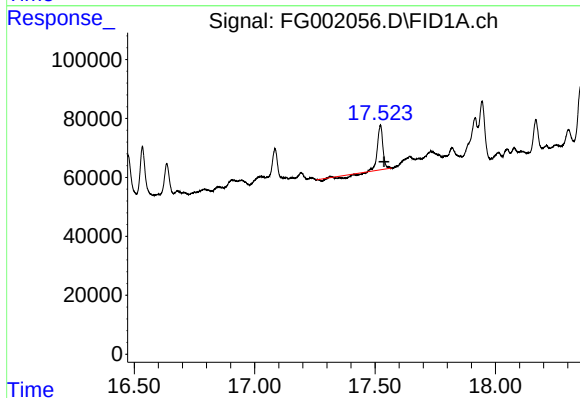


#13 N-TRIACONTANE

R.T.: 17.523 min
Delta R.T.: -0.015 min
Response: 196101
Conc: 1.44 ug/ml

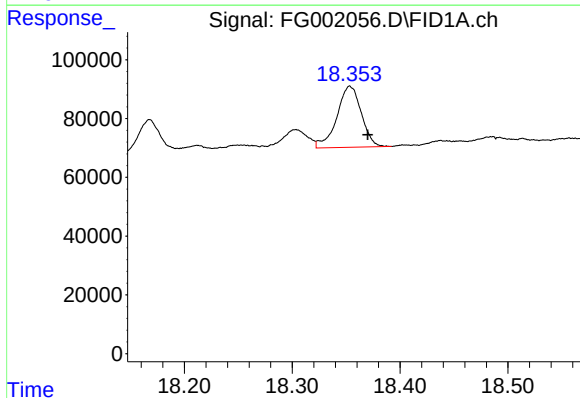


#14 N-DOTRIACONTANE

R.T.: 18.353 min
Delta R.T.: -0.017 min
Response: 326961
Conc: 2.64 ug/ml

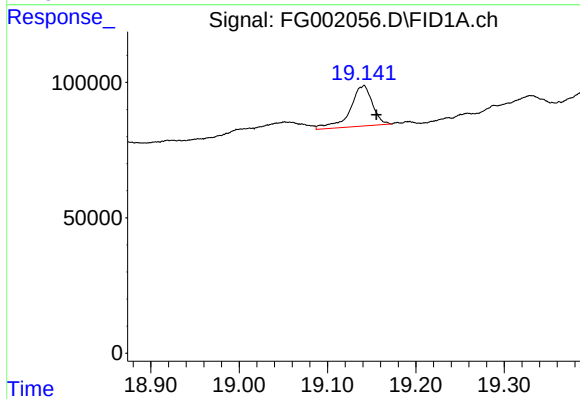

#15 N-TETRATRIACONTANE

R.T.: 19.141 min
Delta R.T.: -0.014 min
Response: 262184
Conc: 2.41 ug/ml

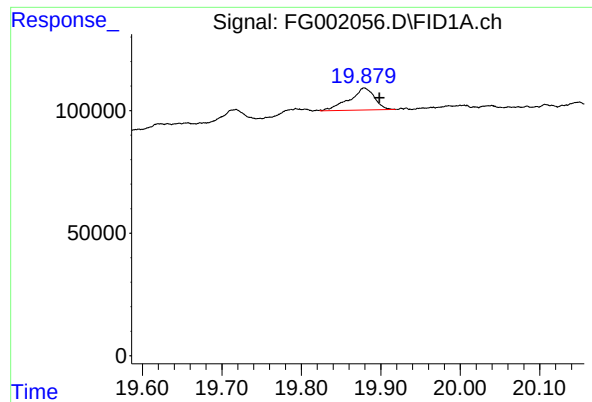

#16 N-HEXATRIACONTANE

R.T.: 19.879 min
Delta R.T.: -0.019 min
Response: 198000
Conc: 2.06 ug/ml

Instrument :
FID_G
ClientSampleId :