

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081018\
Data File : FG002058.D
Signal(s) : FID1A.ch
Acq On : 10 Aug 2018 22:58
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 11 02:21:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG073018.M
Quant Title :
QLast Update : Mon Jul 30 13:56:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.461	1929826	15.310 ug/ml
Target Compounds			
16) N-HEXATRIACONTANE	19.858	22427	0.233 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081018\
Data File : FG002058.D
Signal(s) : FID1A.ch
Acq On : 10 Aug 2018 22:58
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 11 02:21:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG073018.M
Quant Title :
QLast Update : Mon Jul 30 13:56:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

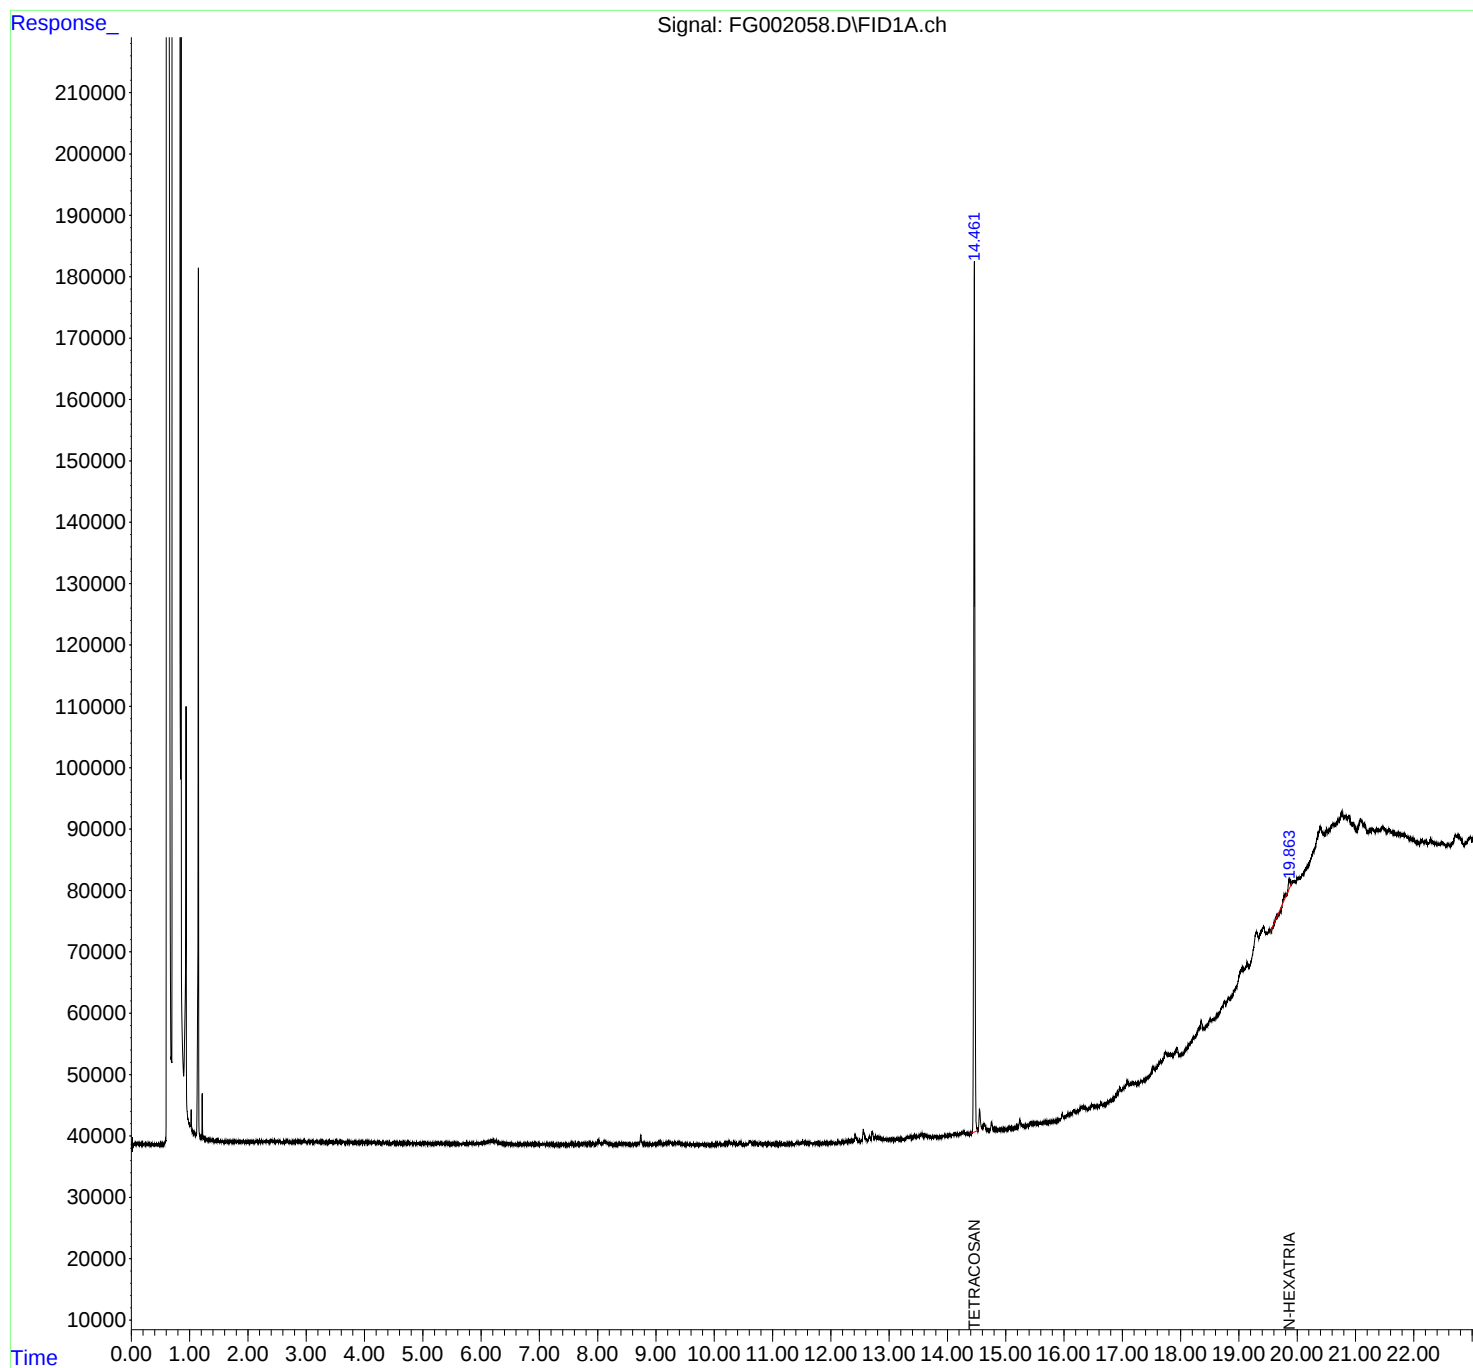


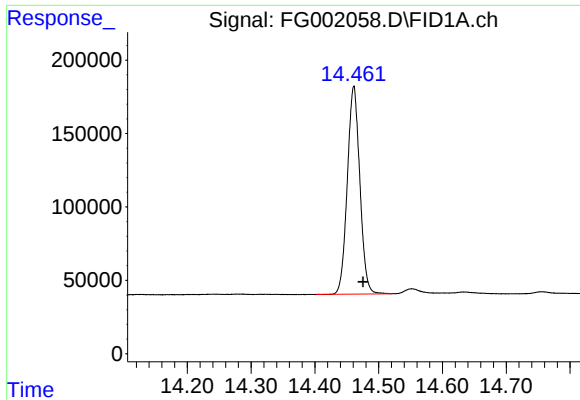

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.461 min
Delta R.T.: -0.014 min
Response: 1929826
Conc: 15.31 ug/ml

Instrument :
FID_G
ClientSampleId :

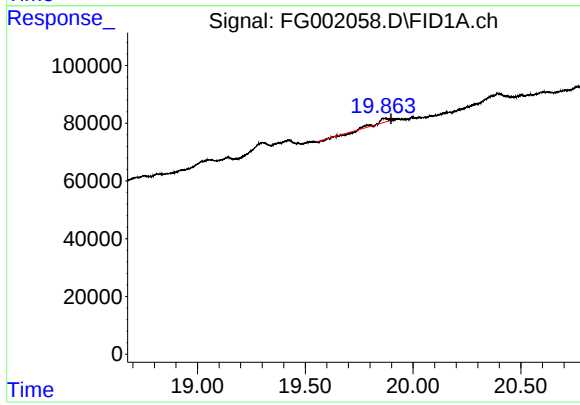

#16 N-HEXATRIACONTANE

R.T.: 19.858 min
Delta R.T.: -0.040 min
Response: 22427
Conc: 0.23 ug/ml