

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081121\
 Data File : FG008590.D
 Signal(s) : FID1A.ch
 Acq On : 11 Aug 2021 16:04
 Operator : DD\AJ
 Sample : M3353-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 12 01:38:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG071521.M
 Quant Title :
 QLast Update : Thu Jul 15 13:17:03 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.759	1834853	12.877 ug/ml
Target Compounds			
7) N-EICOSANE	12.723f	423936	2.601 ug/ml
10) N-TETRACOSANE	14.951	241725	1.474 ug/ml
14) N-DOTRIACONTANE	18.656	220827	1.470 ug/ml
15) N-TETRATRIACONTANE	19.521f	178993	1.299 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081121\
Data File : FG008590.D
Signal(s) : FID1A.ch
Acq On : 11 Aug 2021 16:04
Operator : DD\AJ
Sample : M3353-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 12 01:38:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG071521.M
Quant Title :
QLast Update : Thu Jul 15 13:17:03 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

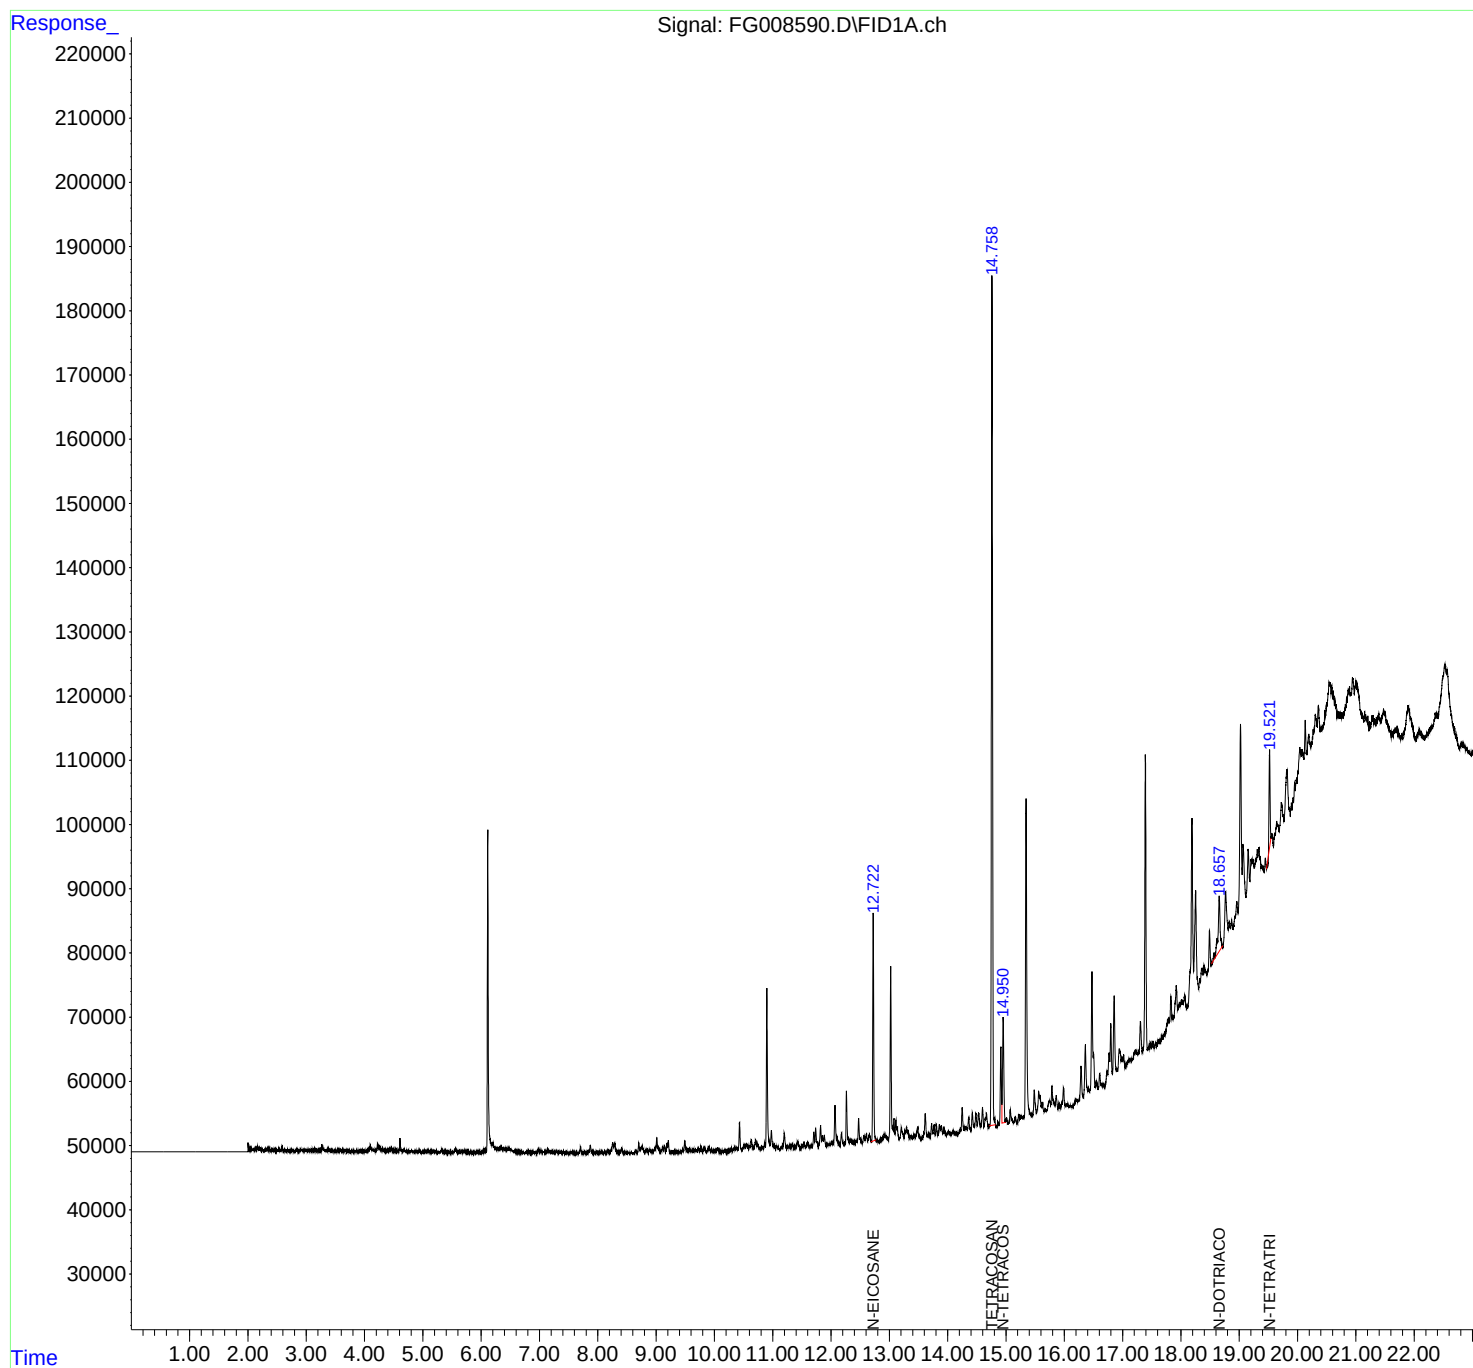


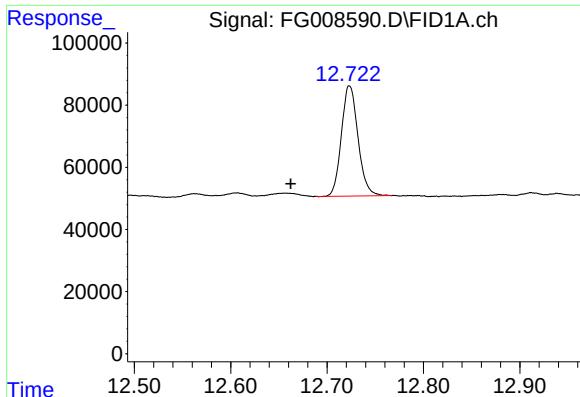

#7 N-EICOSANE


R.T.: 12.723 min
Delta R.T.: 0.061 min
Response: 423936
Conc: 2.60 ug/ml

Instrument :
FID_G
ClientSampleId :

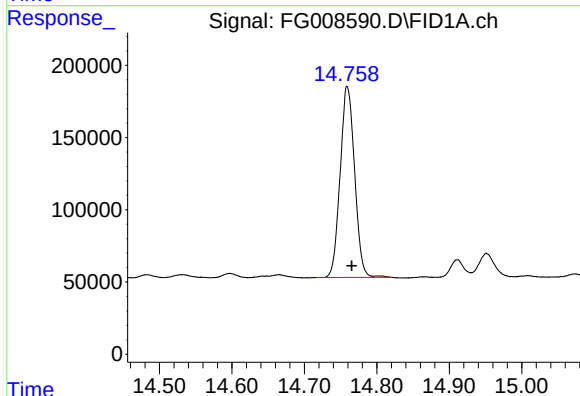


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.759 min
Delta R.T.: -0.006 min
Response: 1834853
Conc: 12.88 ug/ml

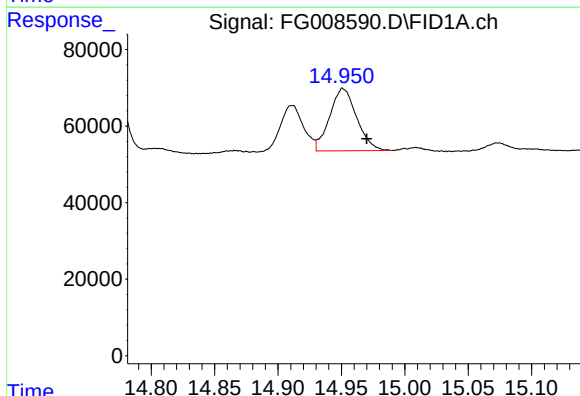


#10 N-TETRACOSANE

R.T.: 14.951 min
Delta R.T.: -0.019 min
Response: 241725
Conc: 1.47 ug/ml

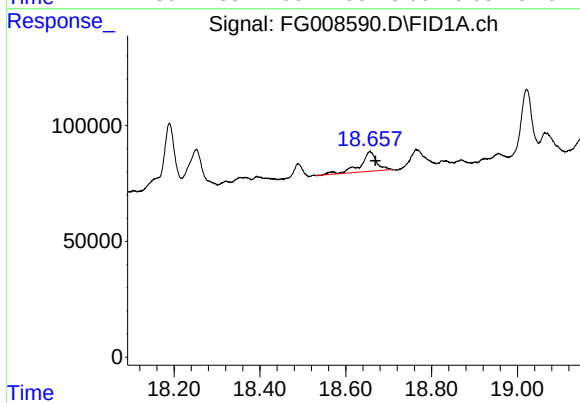

#14 N-DOTRIACONTANE

R.T.: 18.656 min
Delta R.T.: -0.013 min
Response: 220827
Conc: 1.47 ug/ml

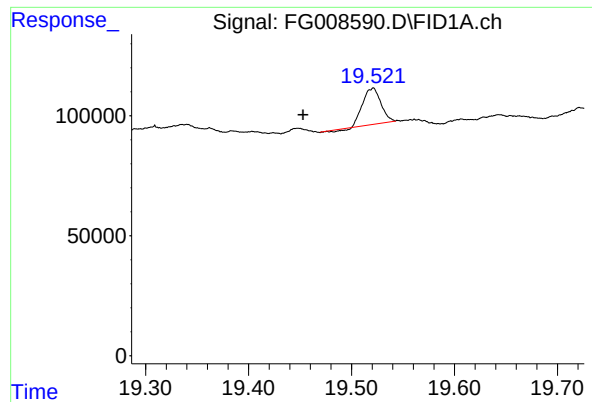

#15 N-TETRATRIACONTANE

R.T.: 19.521 min

Delta R.T.: 0.068 min

Response: 178993

Conc: 1.30 ug/ml

Instrument :
FID_G
ClientSampleId :