

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081121\
 Data File : FG008593.D
 Signal(s) : FID1A.ch
 Acq On : 11 Aug 2021 17:40
 Operator : DD\AJ
 Sample : M3324-01 2X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 12 01:38:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG071521.M
 Quant Title :
 QLast Update : Thu Jul 15 13:17:03 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.761	901360	6.326 ug/ml
Target Compounds			
7) N-EICOSANE	12.725f	97335	0.597 ug/ml
10) N-TETRACOSANE	14.955	132743	0.809 ug/ml
12) N-OCTACOSANE	16.990	117936	0.736 ug/ml
13) N-TRIACONTANE	17.831	255874	1.619 ug/ml
14) N-DOTRIACONTANE	18.658	444860	2.961 ug/ml
15) N-TETRATRIACONTANE	19.448	110388	0.801 ug/ml
16) N-HEXATRIACONTANE	20.193	98441	0.835 ug/ml
17) N-OCTATRIACONTANE	20.948	475378	4.765 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081121\
Data File : FG008593.D
Signal(s) : FID1A.ch
Acq On : 11 Aug 2021 17:40
Operator : DD\AJ
Sample : M3324-01 2X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_G
ClientSampled :

Integration File: autoint1.e
Quant Time: Aug 12 01:38:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG071521.M
Quant Title :
QLast Update : Thu Jul 15 13:17:03 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

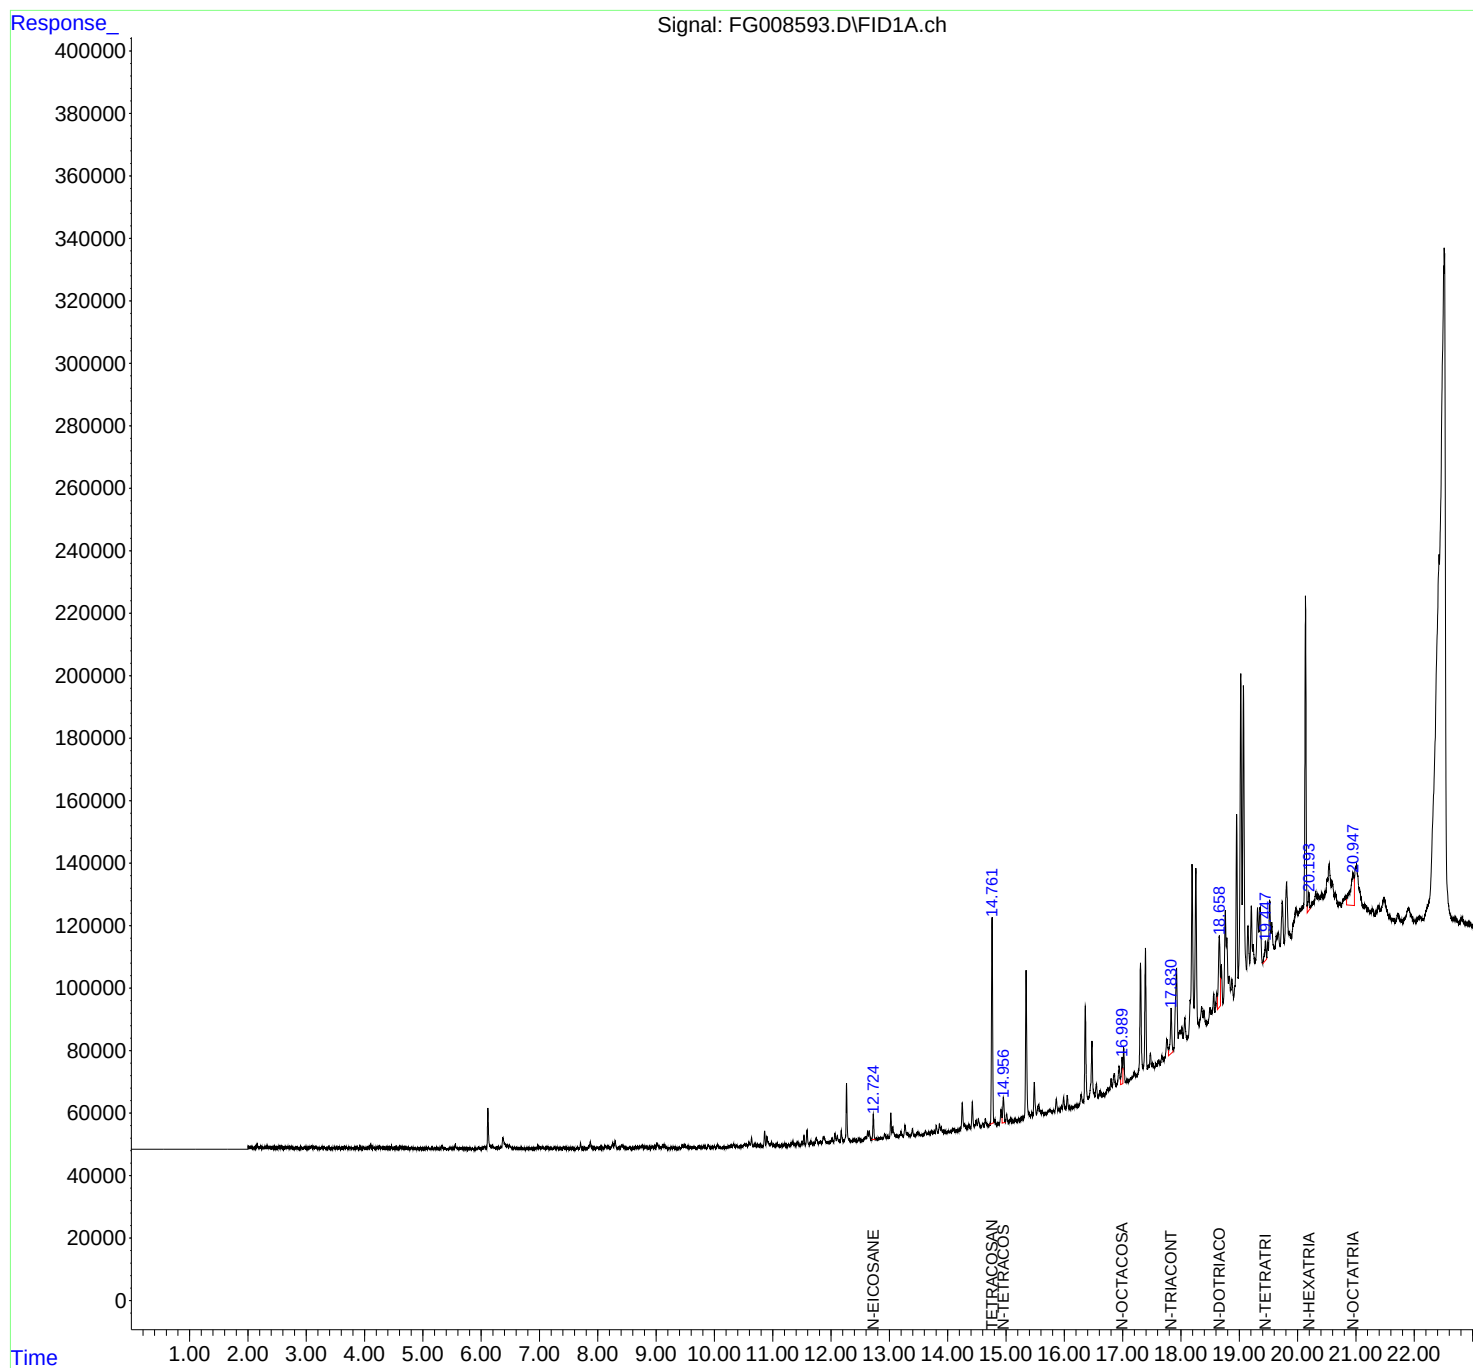


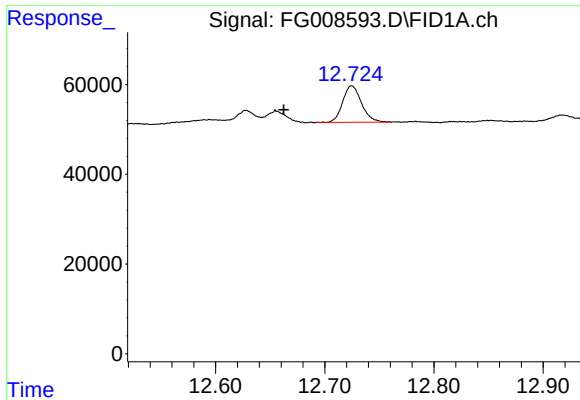

#7 N-EICOSANE


R.T.: 12.725 min
Delta R.T.: 0.062 min
Response: 97335
Conc: 0.60 ug/ml

Instrument :
FID_G
ClientSampleId :

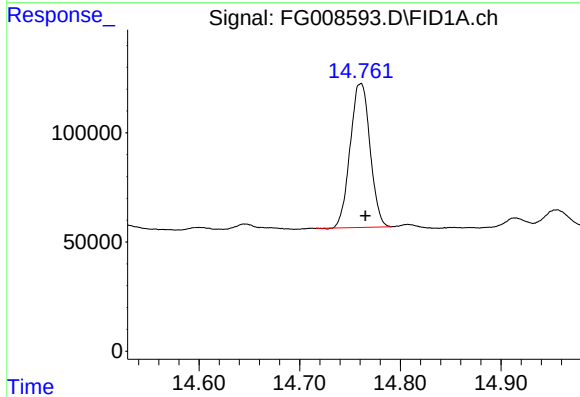


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.761 min
Delta R.T.: -0.005 min
Response: 901360
Conc: 6.33 ug/ml

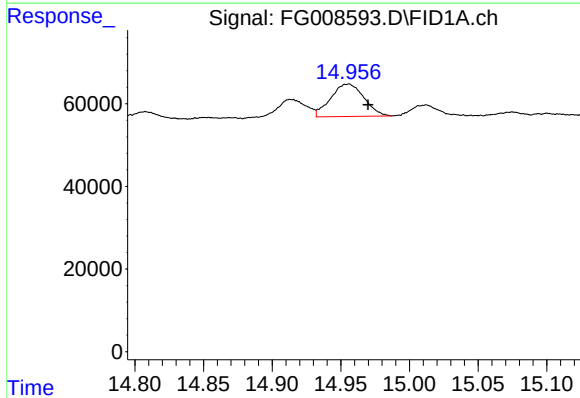


#10 N-TETRACOSANE

R.T.: 14.955 min
Delta R.T.: -0.015 min
Response: 132743
Conc: 0.81 ug/ml

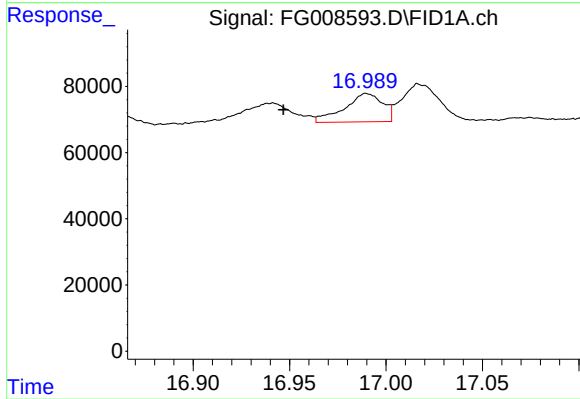

#12 N-OCTACOSANE


R.T.: 16.990 min
Delta R.T.: 0.043 min
Response: 117936
Conc: 0.74 ug/ml

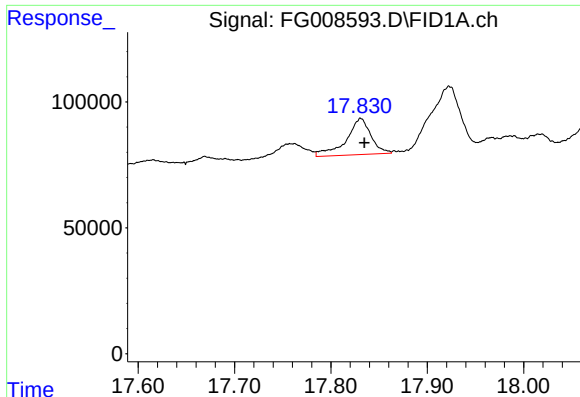

#13 N-TRIACONTANE


R.T.: 17.831 min
Delta R.T.: -0.003 min
Response: 255874
Conc: 1.62 ug/ml

Instrument :
FID_G
ClientSampleId :

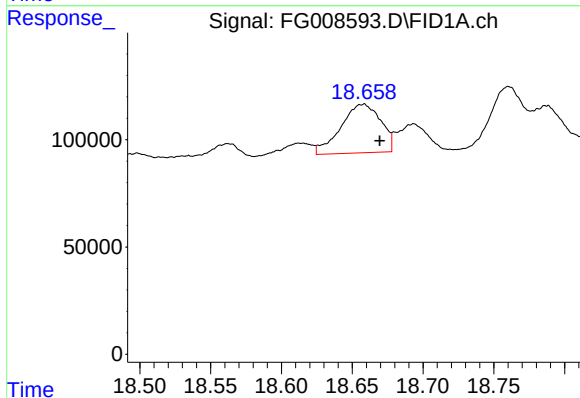


#14 N-DOTRIACONTANE

R.T.: 18.658 min
Delta R.T.: -0.012 min
Response: 444860
Conc: 2.96 ug/ml

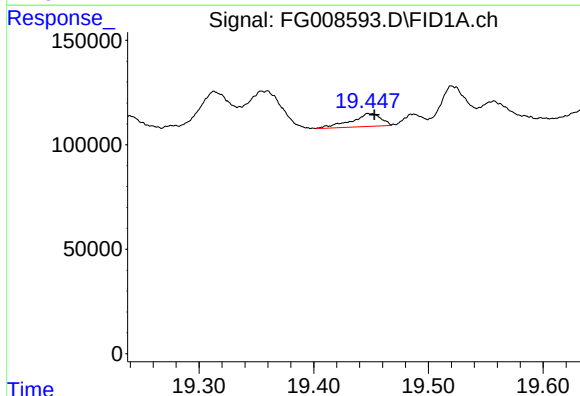


#15 N-TETRATRIACONTANE

R.T.: 19.448 min
Delta R.T.: -0.005 min
Response: 110388
Conc: 0.80 ug/ml

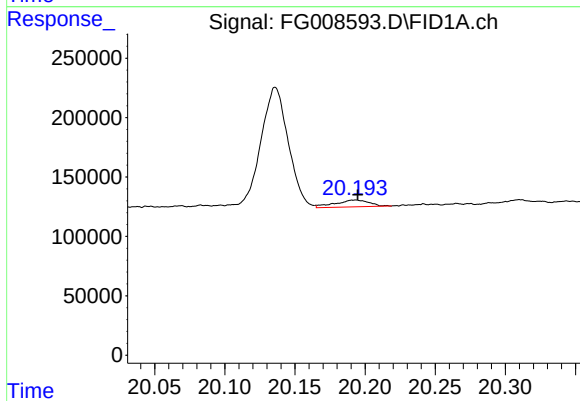

#16 N-HEXATRIACONTANE

R.T.: 20.193 min
Delta R.T.: -0.002 min
Response: 98441
Conc: 0.84 ug/ml

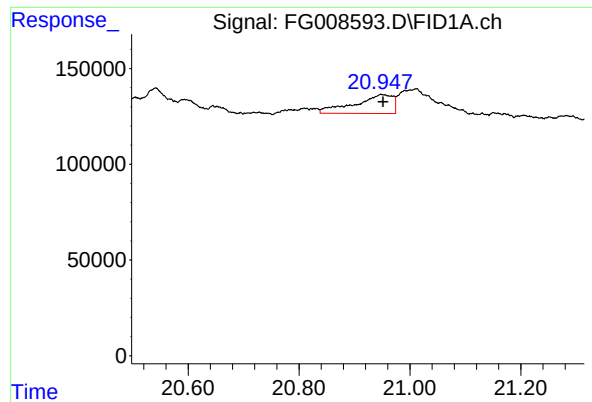

#17 N-OCTATRIACONTANE

R.T.: 20.948 min
Delta R.T.: -0.004 min
Response: 475378
Conc: 4.76 ug/ml

Instrument :
FID_G
ClientSampleId :