

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081121\
 Data File : FG008596.D
 Signal(s) : FID1A.ch
 Acq On : 11 Aug 2021 19:16
 Operator : DD\AJ
 Sample : M3331-13 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 12 01:39:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG071521.M
 Quant Title :
 QLast Update : Thu Jul 15 13:17:03 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.759	387319	2.718 ug/ml
Target Compounds			
7) N-EICOSANE	12.724f	119145	0.731 ug/ml
10) N-TETRACOSANE	14.951	267532	1.631 ug/ml
16) N-HEXATRIACONTANE	20.229	956551	8.118 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081121\
Data File : FG008596.D
Signal(s) : FID1A.ch
Acq On : 11 Aug 2021 19:16
Operator : DD\AJ
Sample : M3331-13 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_G
ClientSampled :

Integration File: autoint1.e
Quant Time: Aug 12 01:39:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG071521.M
Quant Title :
QLast Update : Thu Jul 15 13:17:03 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

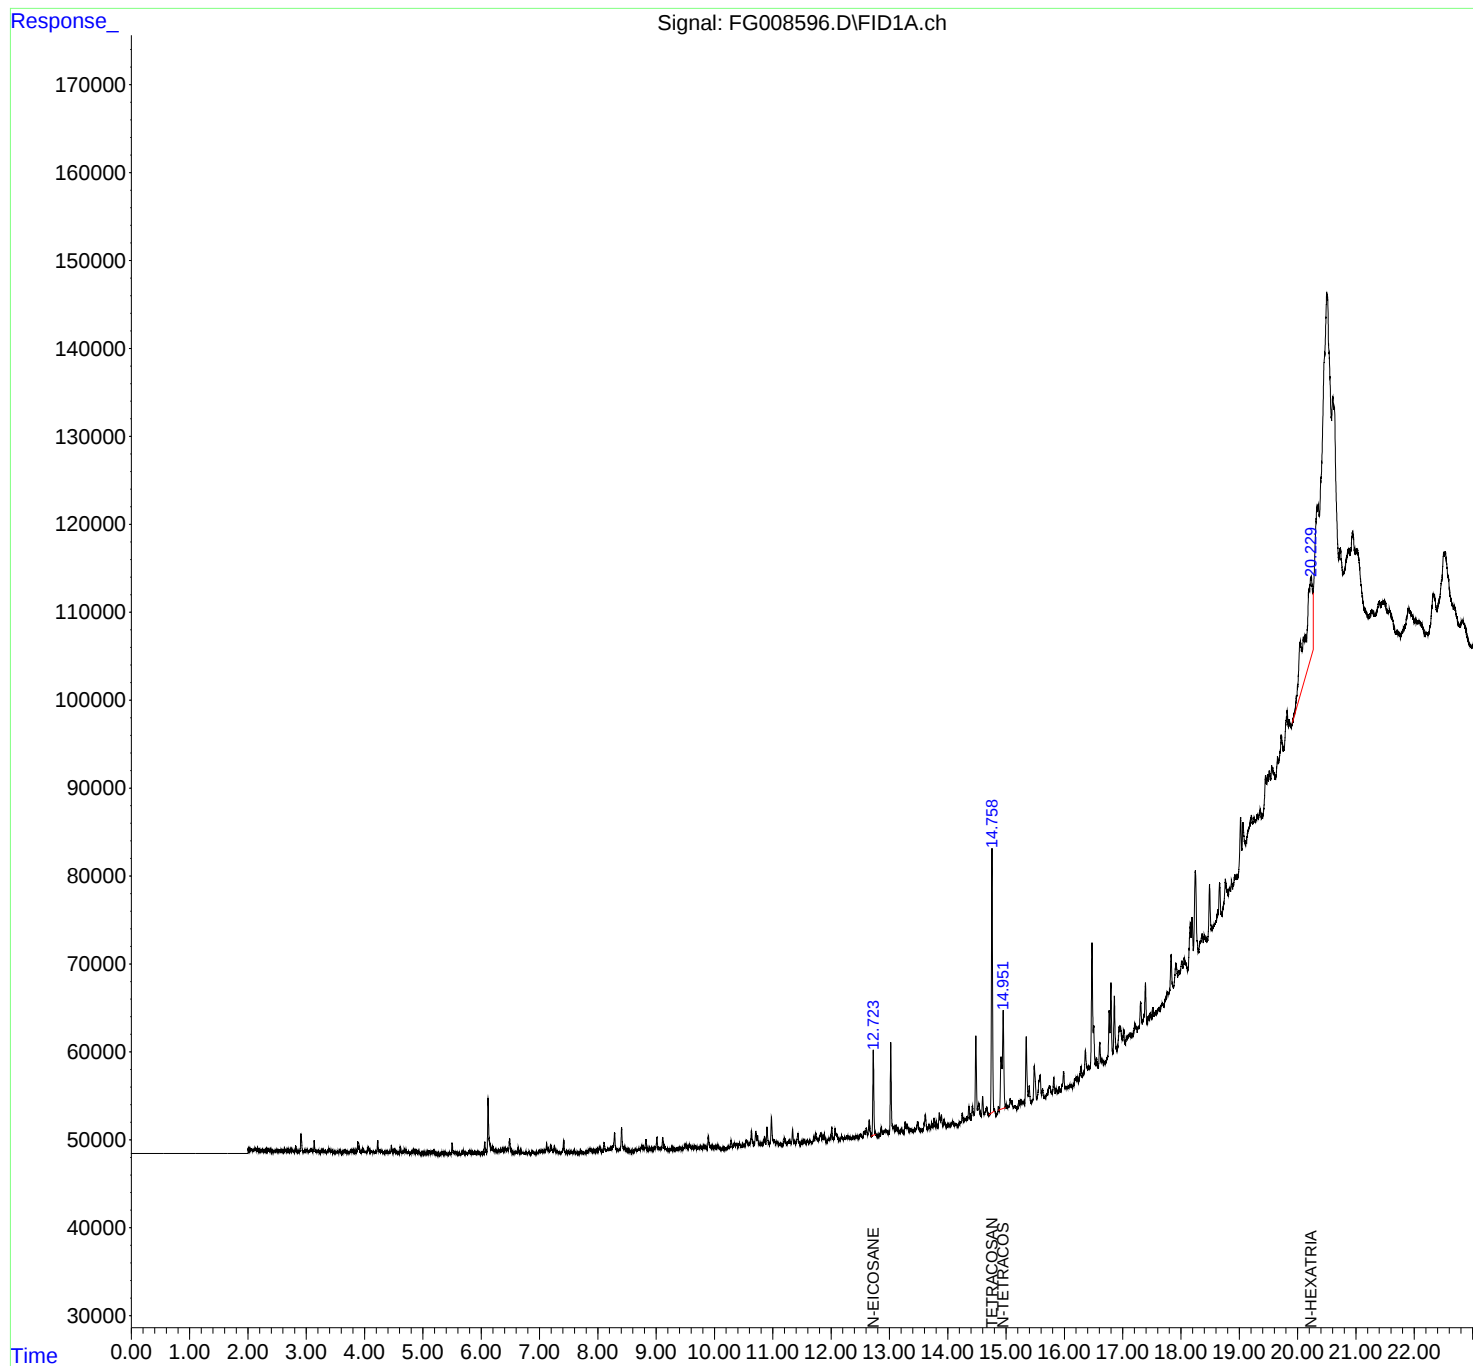


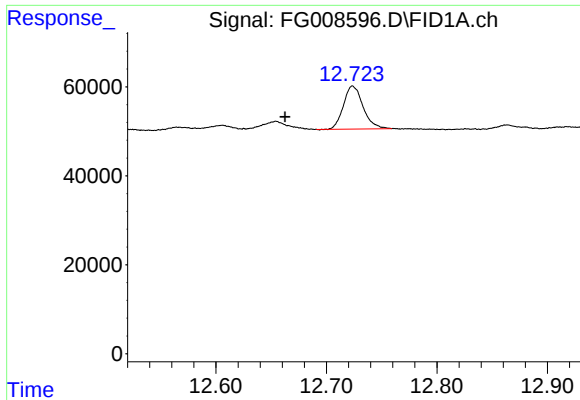

#7 N-EICOSANE


R.T.: 12.724 min
Delta R.T.: 0.061 min
Response: 119145
Conc: 0.73 ug/ml

Instrument :
FID_G
ClientSampleId :

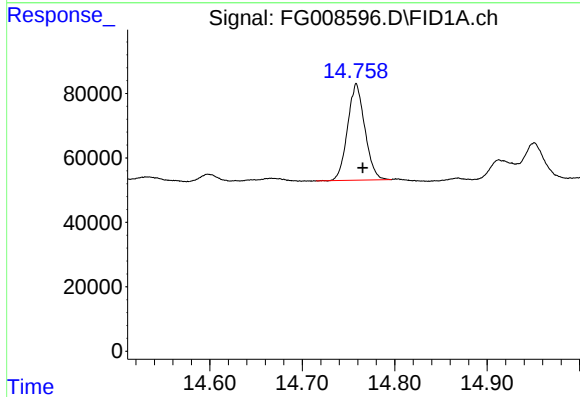


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.759 min
Delta R.T.: -0.007 min
Response: 387319
Conc: 2.72 ug/ml

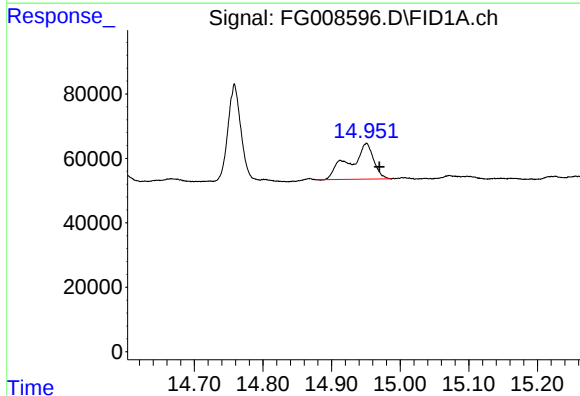

#10 N-TETRACOSANE

R.T.: 14.951 min
Delta R.T.: -0.019 min
Response: 267532
Conc: 1.63 ug/ml

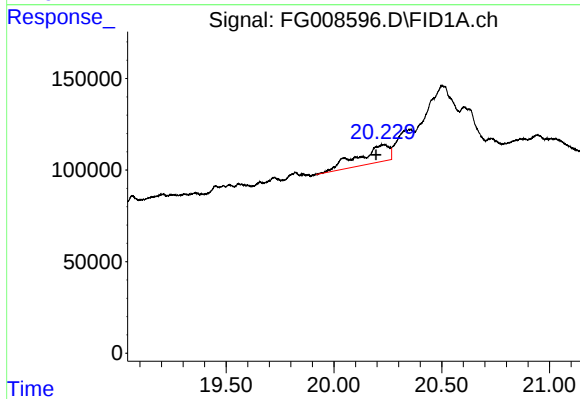

#16 N-HEXATRIACONTANE

R.T.: 20.229 min
Delta R.T.: 0.034 min
Response: 956551
Conc: 8.12 ug/ml