

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081121\
Data File : FG008608.D
Signal(s) : FID1A.ch
Acq On : 12 Aug 2021 01:36
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 12 03:15:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG071521.M
Quant Title :
QLast Update : Thu Jul 15 13:17:03 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14)	N-DOTRIACONTANE	18.662	180199	1.199 ug/ml
16)	N-HEXATRIACONTANE	20.200	131233	1.114 ug/ml
17)	N-OCTATRIACONTANE	20.894f	17756	0.178 ug/ml
18)	N-TETRACONTANE	21.915	279088	3.080 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081121\
Data File : FG008608.D
Signal(s) : FID1A.ch
Acq On : 12 Aug 2021 01:36
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 12 03:15:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG071521.M
Quant Title :
QLast Update : Thu Jul 15 13:17:03 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

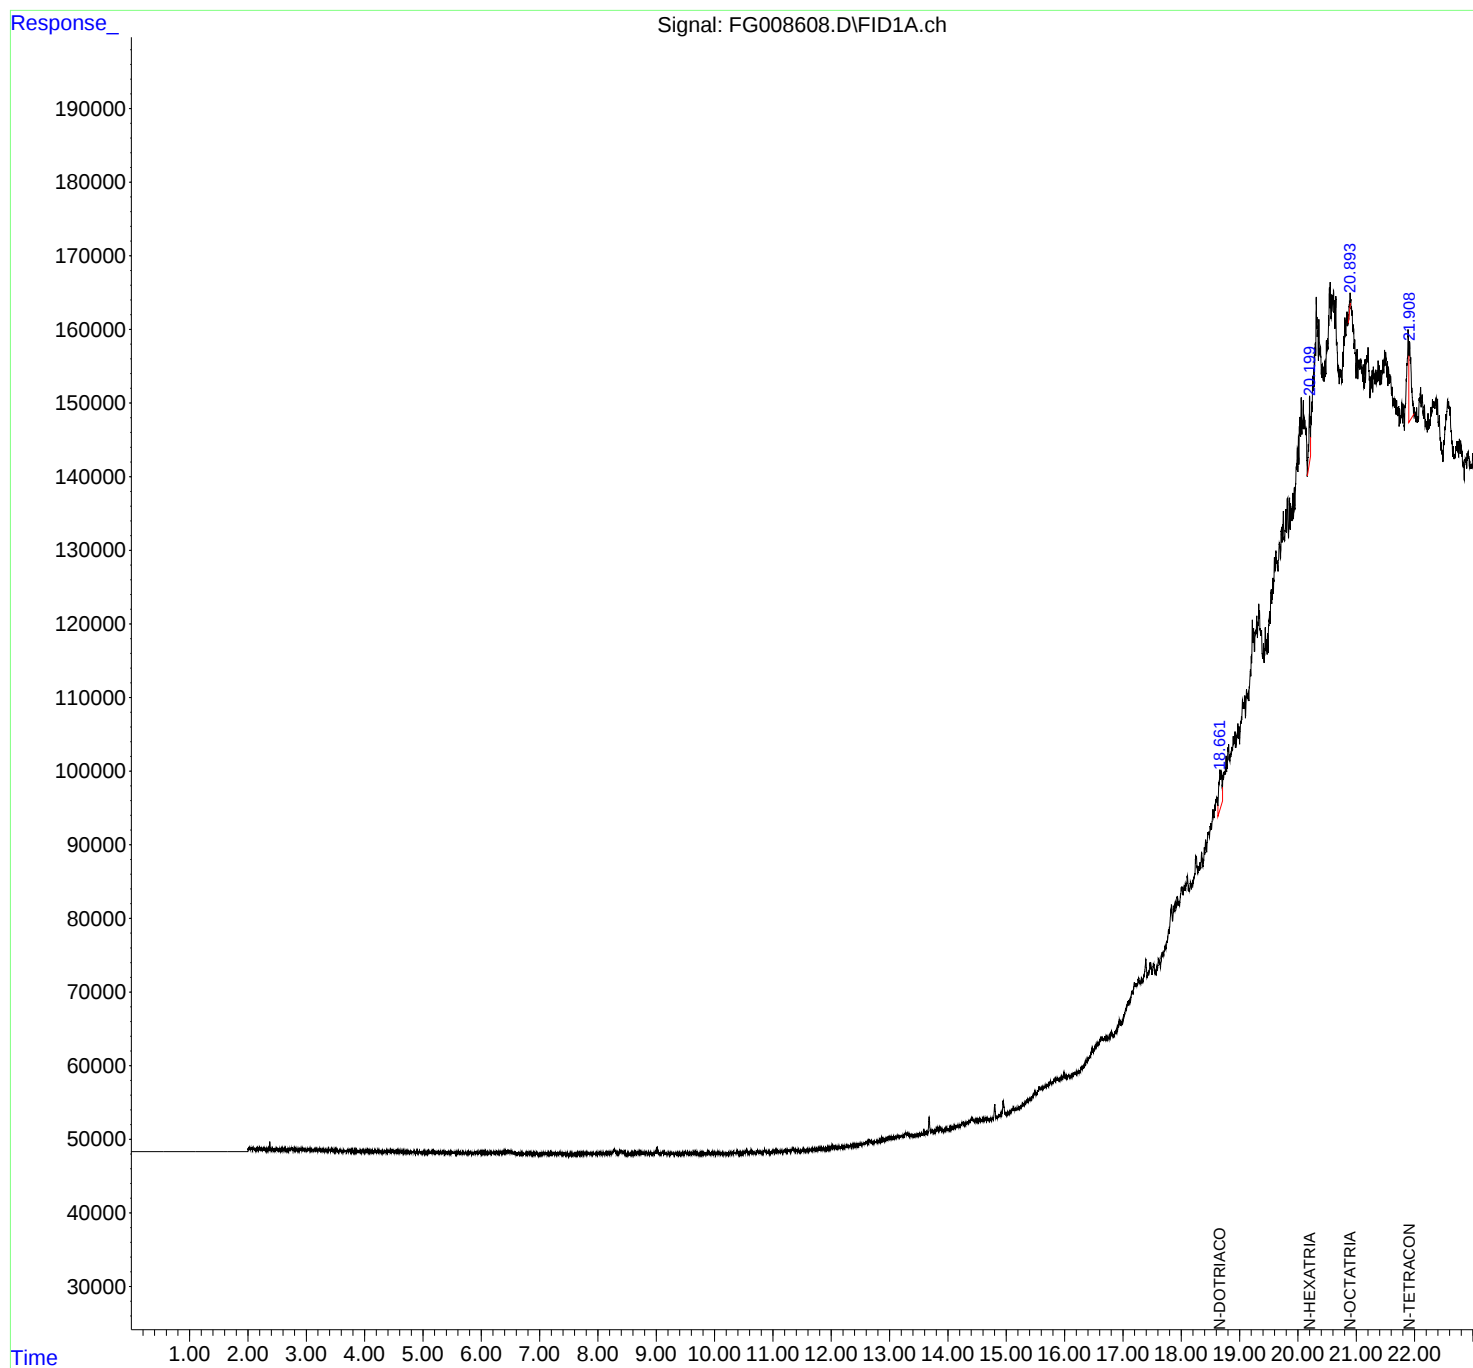


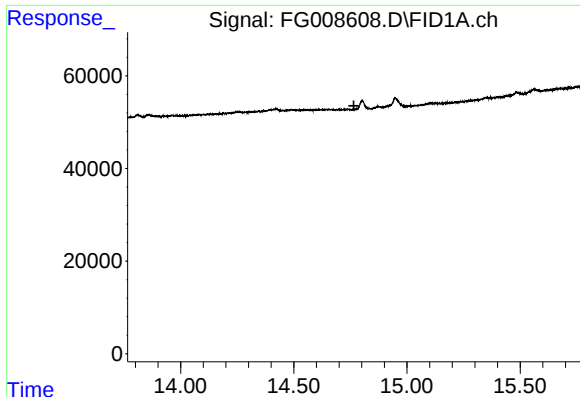

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.765 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

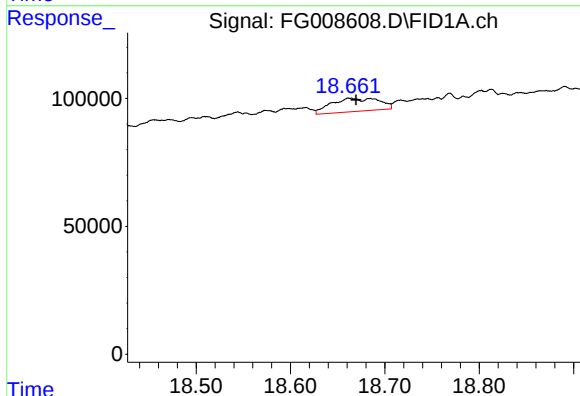


#14 N-DOTRIACONTANE

R.T.: 18.662 min
Delta R.T.: -0.007 min
Response: 180199
Conc: 1.20 ug/ml

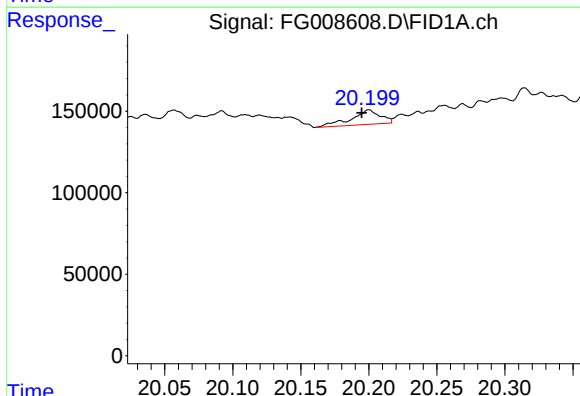


#16 N-HEXATRIACONTANE

R.T.: 20.200 min
Delta R.T.: 0.005 min
Response: 131233
Conc: 1.11 ug/ml

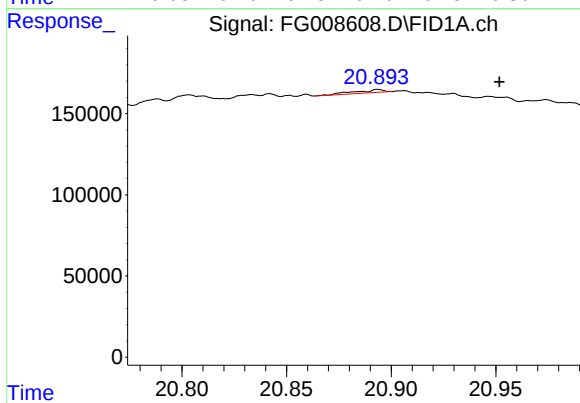

#17 N-OCTATRIACONTANE

R.T.: 20.894 min
Delta R.T.: -0.058 min
Response: 17756
Conc: 0.18 ug/ml

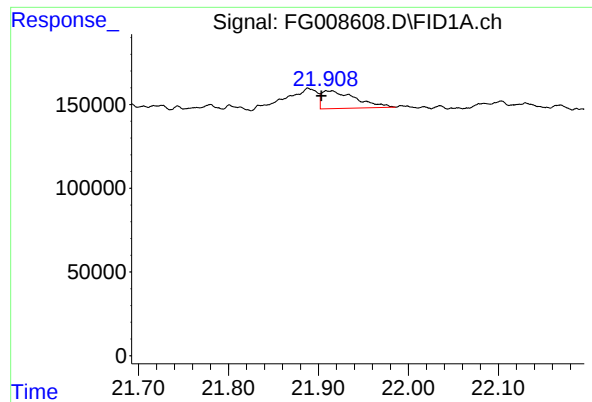

#18 N-TETRACONTANE

R.T.: 21.915 min
Delta R.T.: 0.012 min
Response: 279088
Conc: 3.08 ug/ml

Instrument :
FID_G
ClientSampleId :