

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081121\
Data File : FG008603.D
Signal(s) : FID1A.ch
Acq On : 11 Aug 2021 22:59
Operator : DD\AJ
Sample : PB138323BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB138323BL

Integration File: autoint1.e
Quant Time: Aug 12 01:40:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG071521.M
Quant Title :
QLast Update : Thu Jul 15 13:17:03 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.757	2632494	18.475 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081121\
Data File : FG008603.D
Signal(s) : FID1A.ch
Acq On : 11 Aug 2021 22:59
Operator : DD\AJ
Sample : PB138323BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB138323BL

Integration File: autoint1.e
Quant Time: Aug 12 01:40:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG071521.M
Quant Title :
QLast Update : Thu Jul 15 13:17:03 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

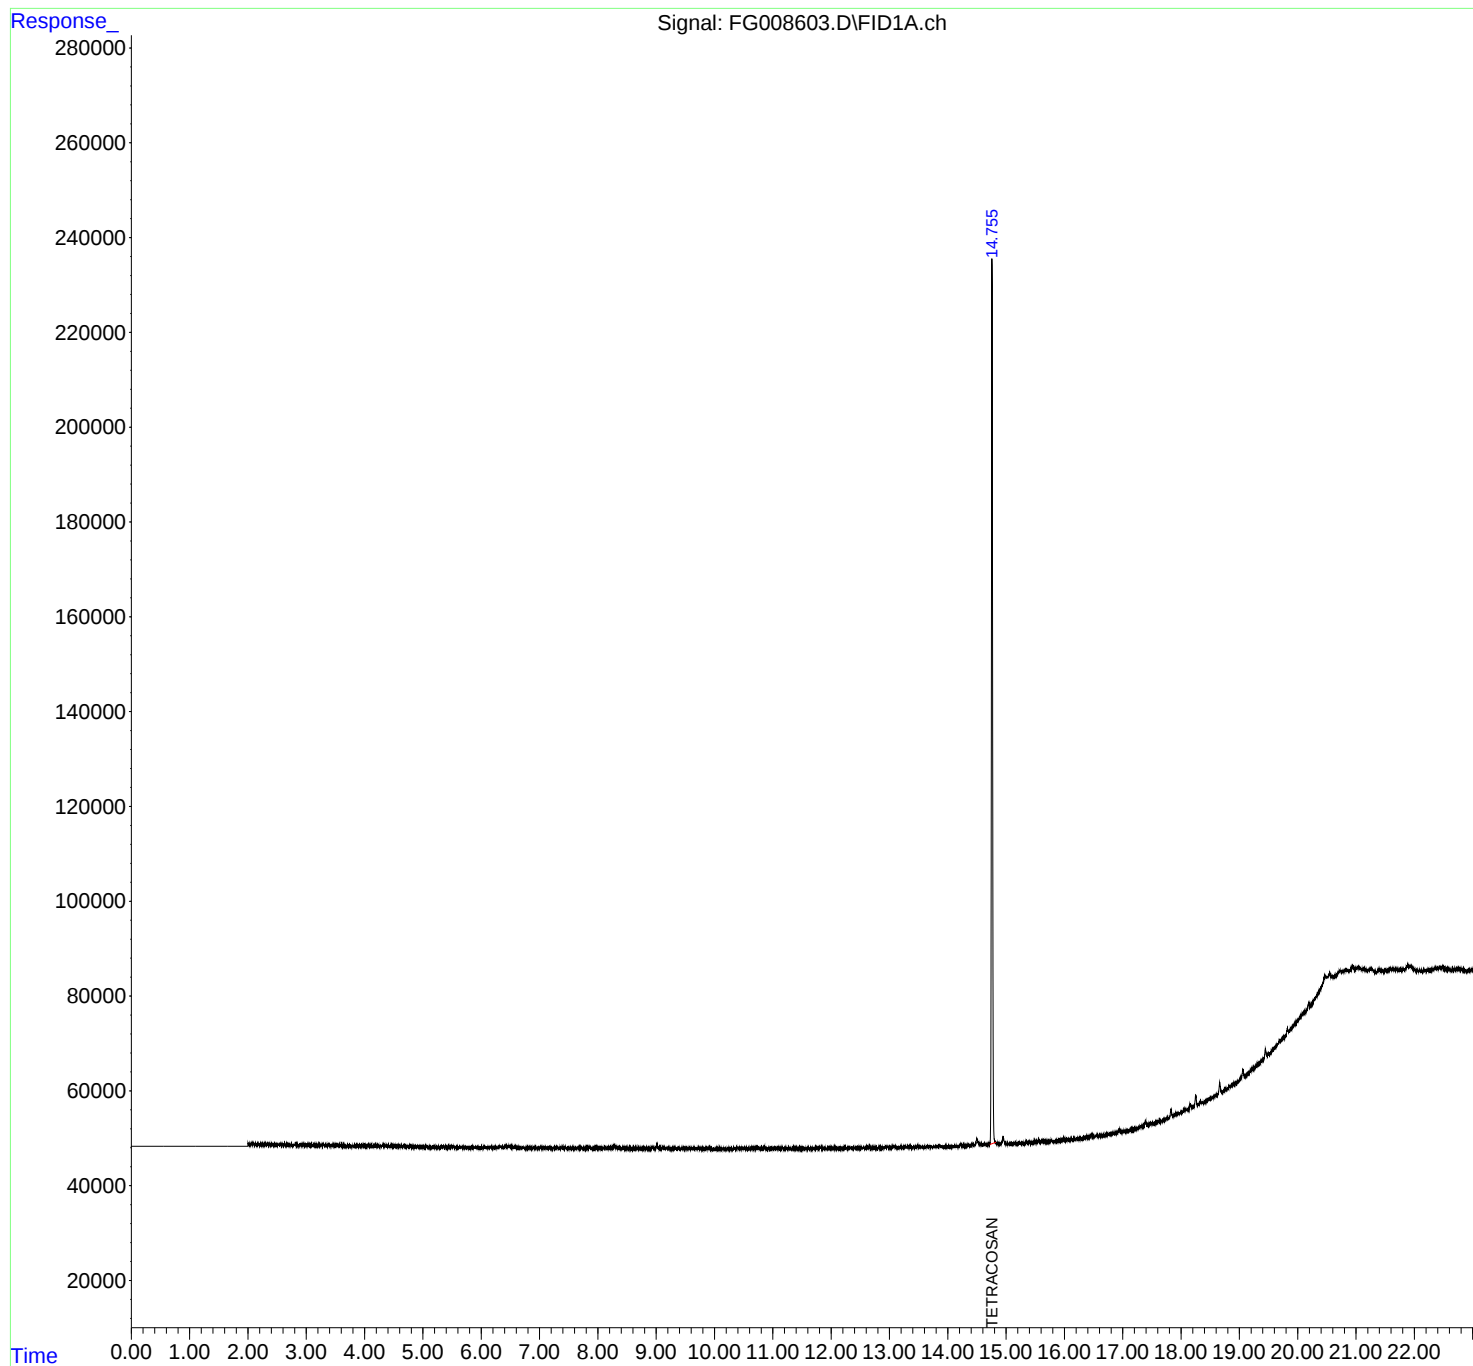

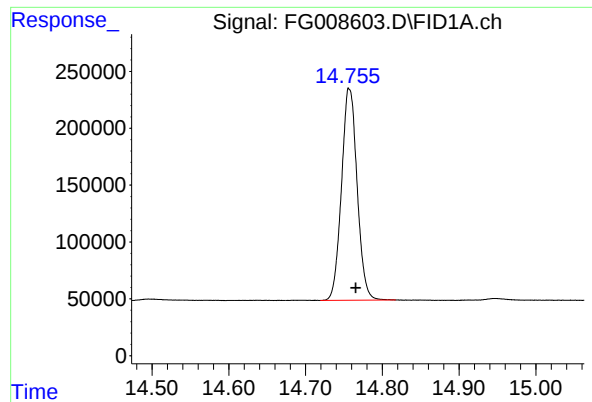

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.757 min
Delta R.T.: -0.009 min
Response: 2632494
Conc: 18.47 ug/ml

Instrument :
FID_G
ClientSampleId :
PB138323BL