

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081122\
Data File : FG010344.D
Signal(s) : FID1A.ch
Acq On : 11 Aug 2022 16:38
Operator : YP\AJ
Sample : N4082-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
CRUSHED-MASONARY-PILE-A

Integration File: autoint1.e
Quant Time: Aug 12 04:50:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG072822.M
Quant Title :
QLast Update : Thu Jul 28 15:10:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.794	1423919	11.209 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081122\
Data File : FG010344.D
Signal(s) : FID1A.ch
Acq On : 11 Aug 2022 16:38
Operator : YP\AJ
Sample : N4082-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
CRUSHED-MASONARY-PILE-A

Integration File: autoint1.e
Quant Time: Aug 12 04:50:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG072822.M
Quant Title :
QLast Update : Thu Jul 28 15:10:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

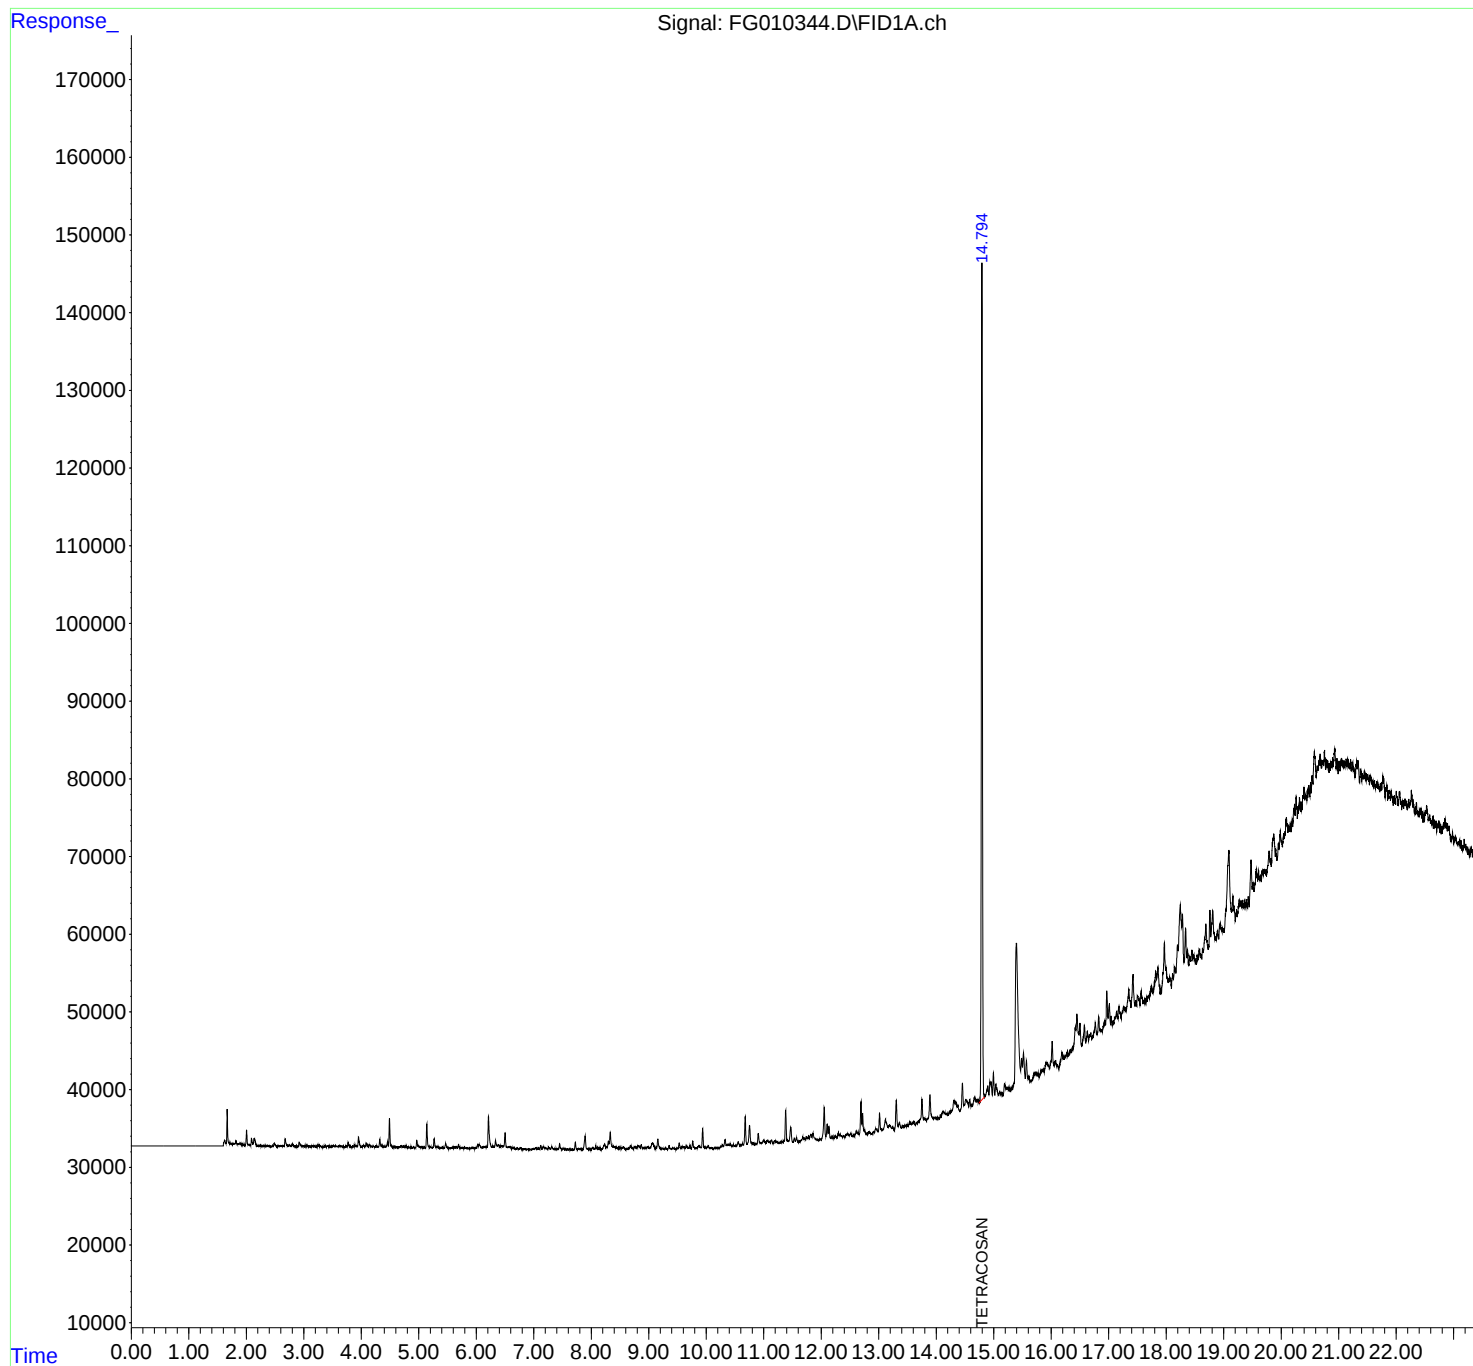

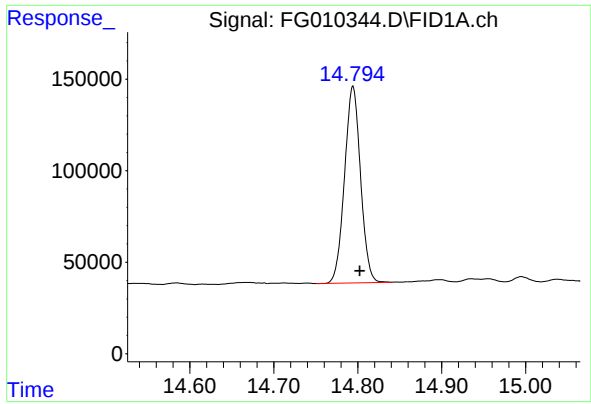

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.794 min
Delta R.T.: -0.008 min
Response: 1423919
Conc: 11.21 ug/ml

Instrument :
FID_G
ClientSampleId :
CRUSHED-MASONARY-PILE-A