

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081321\
 Data File : FG008633.D
 Signal(s) : FID1A.ch
 Acq On : 13 Aug 2021 18:58
 Operator : DD\AJ
 Sample : M3407-26
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 13 22:48:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG071521.M
 Quant Title :
 QLast Update : Thu Jul 15 13:17:03 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.757	2522170	17.700 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.959	157298	0.959 ug/ml
11) N-HEXACOSANE	15.985	148581	0.916 ug/ml
12) N-OCTACOSANE	16.937	125433	0.783 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081321\
Data File : FG008633.D
Signal(s) : FID1A.ch
Acq On : 13 Aug 2021 18:58
Operator : DD\AJ
Sample : M3407-26
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 13 22:48:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG071521.M
Quant Title :
QLast Update : Thu Jul 15 13:17:03 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

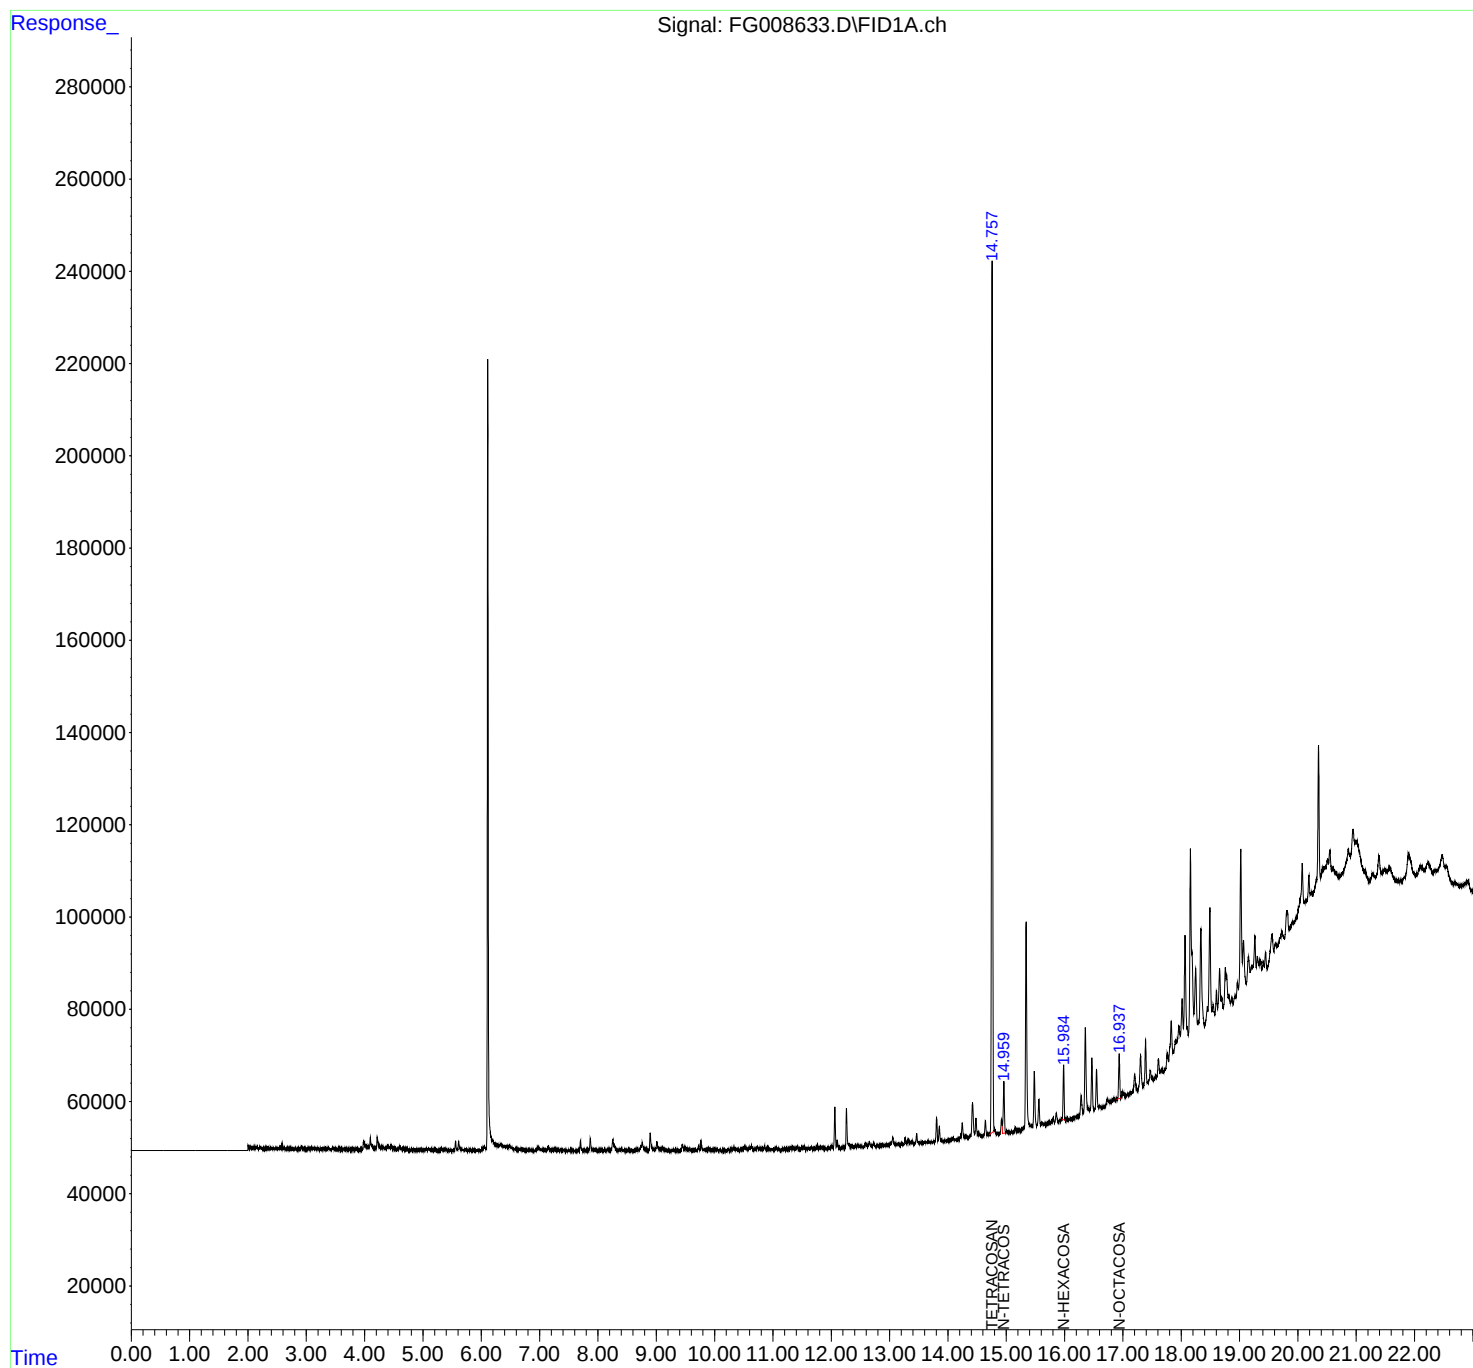


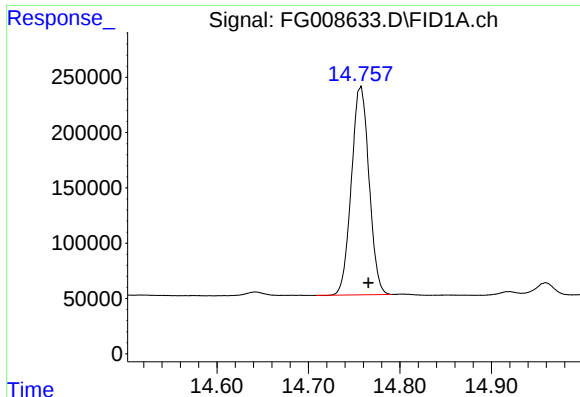

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.757 min
Delta R.T.: -0.009 min
Response: 2522170
Conc: 17.70 ug/ml

Instrument :
FID_G
ClientSampleId :

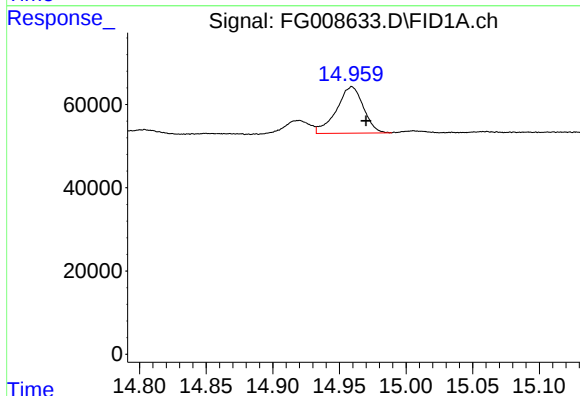


#10 N-TETRACOSANE

R.T.: 14.959 min
Delta R.T.: -0.011 min
Response: 157298
Conc: 0.96 ug/ml

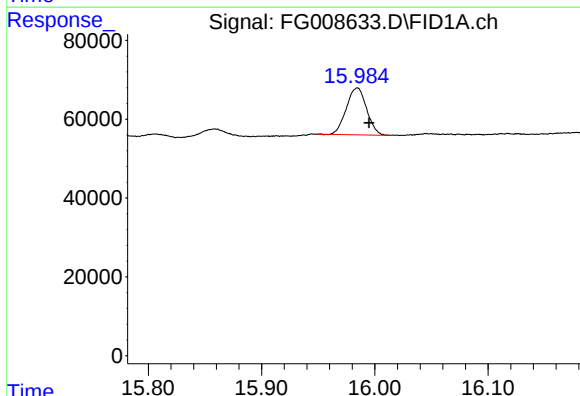

#11 N-HEXACOSANE

R.T.: 15.985 min
Delta R.T.: -0.010 min
Response: 148581
Conc: 0.92 ug/ml

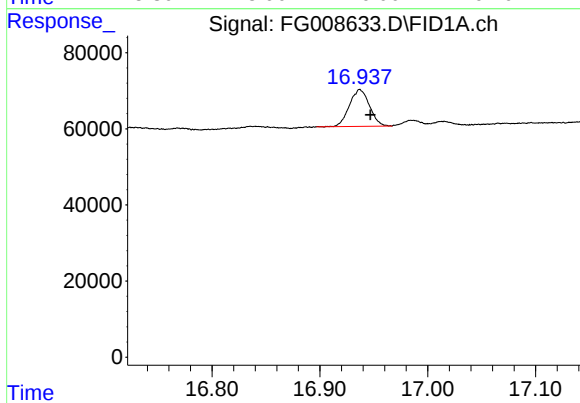

#12 N-OCTACOSANE

R.T.: 16.937 min
Delta R.T.: -0.010 min
Response: 125433
Conc: 0.78 ug/ml