

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081321\
 Data File : FG008635.D
 Signal(s) : FID1A.ch
 Acq On : 13 Aug 2021 20:01
 Operator : DD\AJ
 Sample : M3408-0
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 13 22:49:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG071521.M
 Quant Title :
 QLast Update : Thu Jul 15 13:17:03 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.758	3200037	22.458 ug/ml
Target Compounds			
7) N-EICOSANE	12.720f	777209	4.769 ug/ml
10) N-TETRACOSANE	14.951	496865	3.030 ug/ml
11) N-HEXACOSANE	15.985	178750	1.102 ug/ml
12) N-OCTACOSANE	16.938	166957	1.042 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081321\
Data File : FG008635.D
Signal(s) : FID1A.ch
Acq On : 13 Aug 2021 20:01
Operator : DD\AJ
Sample : M3408-0
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 13 22:49:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG071521.M
Quant Title :
QLast Update : Thu Jul 15 13:17:03 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

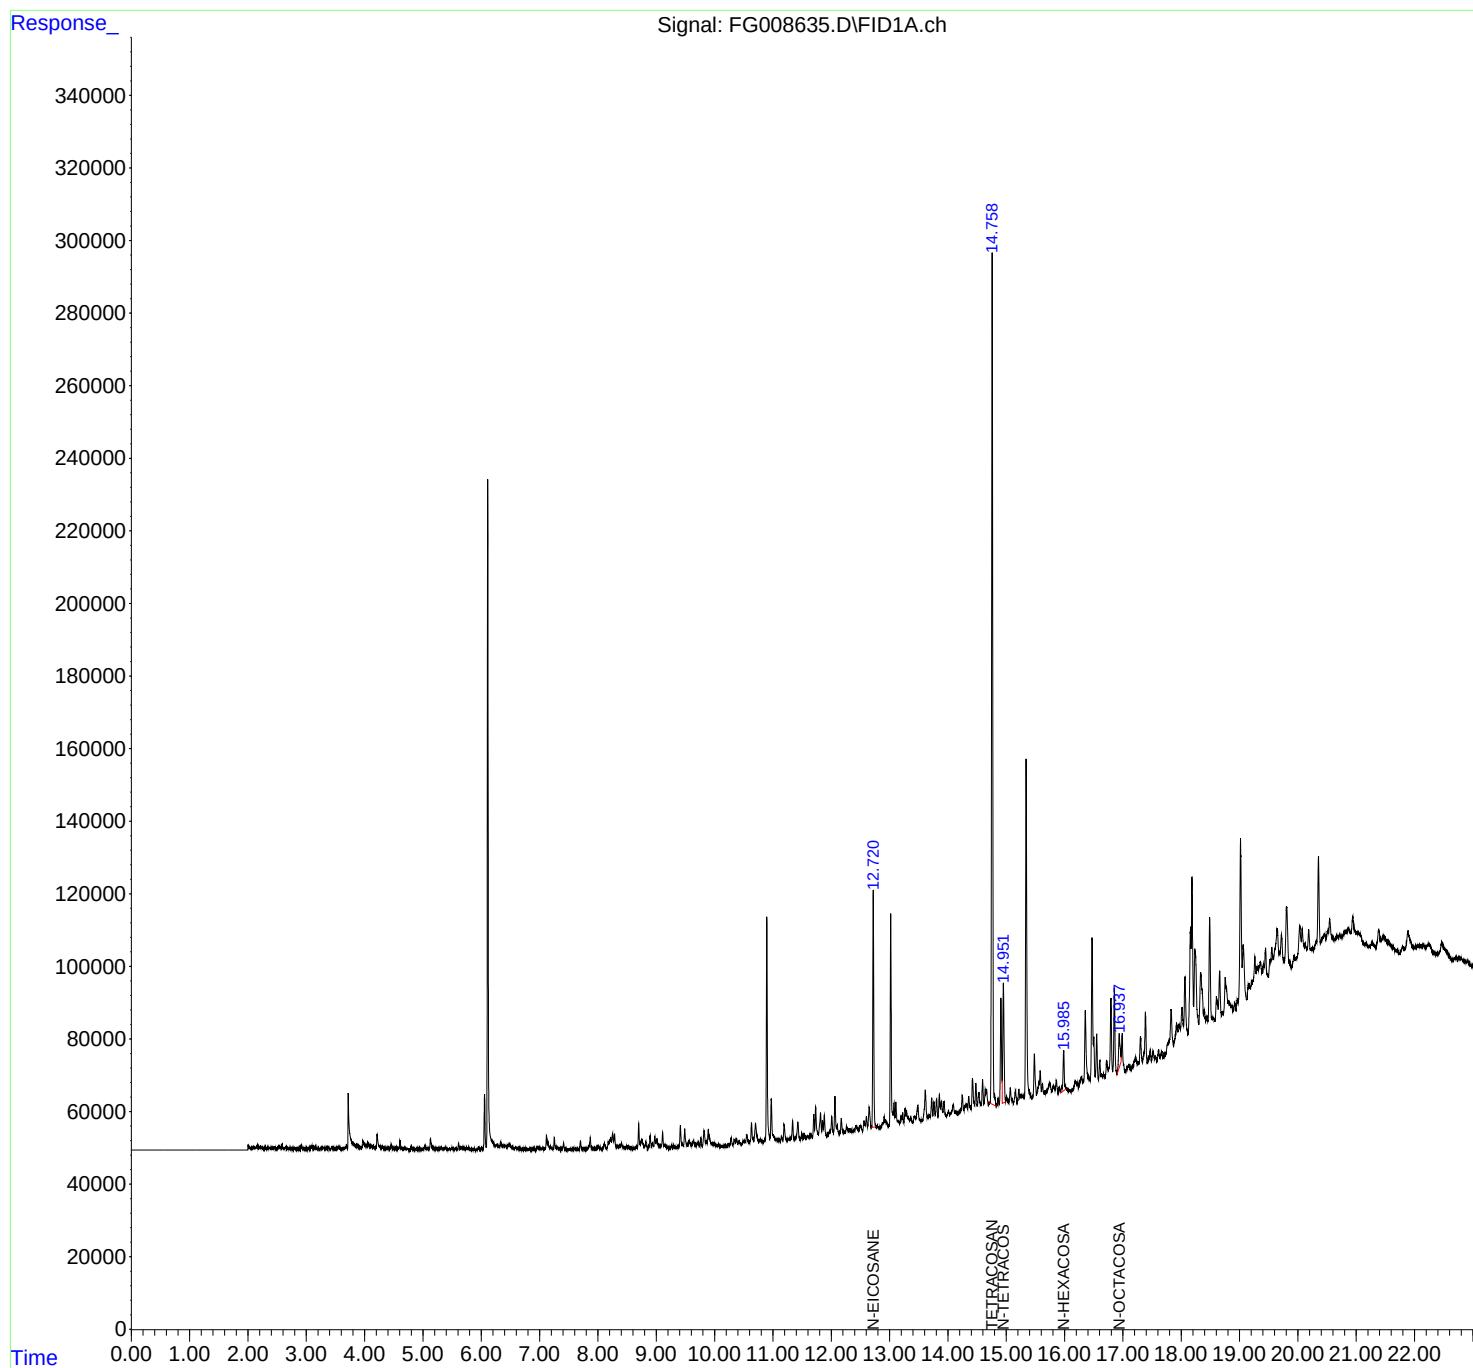


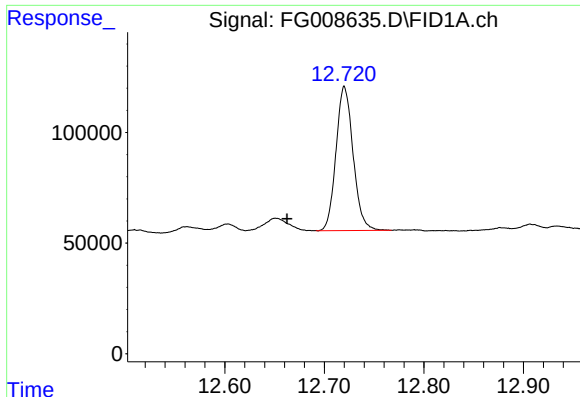

#7 N-EICOSANE


R.T.: 12.720 min
Delta R.T.: 0.058 min
Response: 777209
Conc: 4.77 ug/ml

Instrument :
FID_G
ClientSampleId :

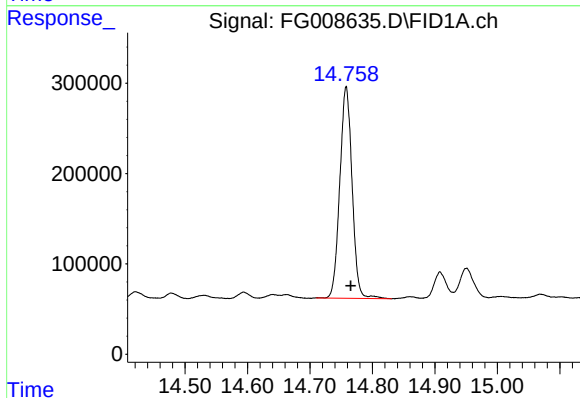


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.758 min
Delta R.T.: -0.008 min
Response: 3200037
Conc: 22.46 ug/ml

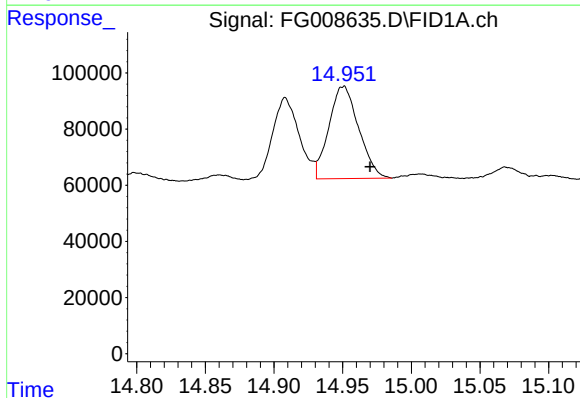


#10 N-TETRACOSANE

R.T.: 14.951 min
Delta R.T.: -0.019 min
Response: 496865
Conc: 3.03 ug/ml

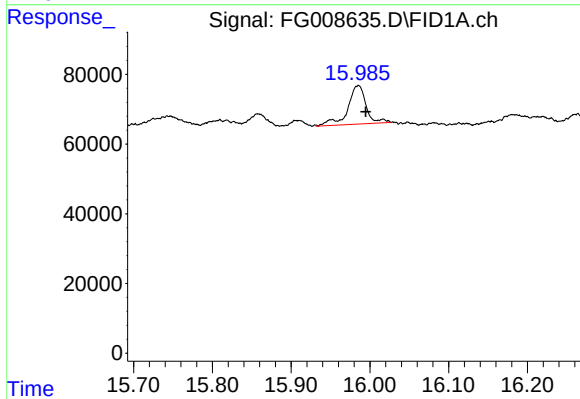

#11 N-HEXACOSANE

R.T.: 15.985 min
Delta R.T.: -0.009 min
Response: 178750
Conc: 1.10 ug/ml

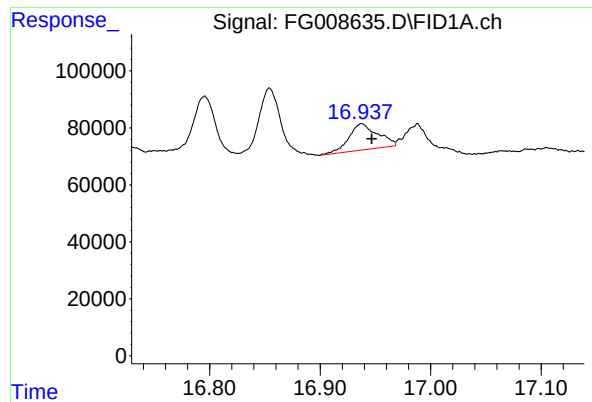

#12 N-OCTACOSANE

R.T.: 16.938 min
Delta R.T.: -0.009 min
Response: 166957
Conc: 1.04 ug/ml

Instrument :
FID_G
ClientSampleId :