

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081321\
 Data File : FG008637.D
 Signal(s) : FID1A.ch
 Acq On : 13 Aug 2021 21:05
 Operator : DD\AJ
 Sample : M3408-11
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 13 22:49:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG071521.M
 Quant Title :
 QLast Update : Thu Jul 15 13:17:03 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.756	2818075	19.777 ug/ml
Target Compounds			
7) N-EICOSANE	12.720f	1125924	6.909 ug/ml
10) N-TETRACOSANE	14.948	640790	3.907 ug/ml
11) N-HEXACOSANE	15.983	196880	1.214 ug/ml
12) N-OCTACOSANE	16.936	218472	1.363 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081321\
Data File : FG008637.D
Signal(s) : FID1A.ch
Acq On : 13 Aug 2021 21:05
Operator : DD\AJ
Sample : M3408-11
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 13 22:49:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG071521.M
Quant Title :
QLast Update : Thu Jul 15 13:17:03 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

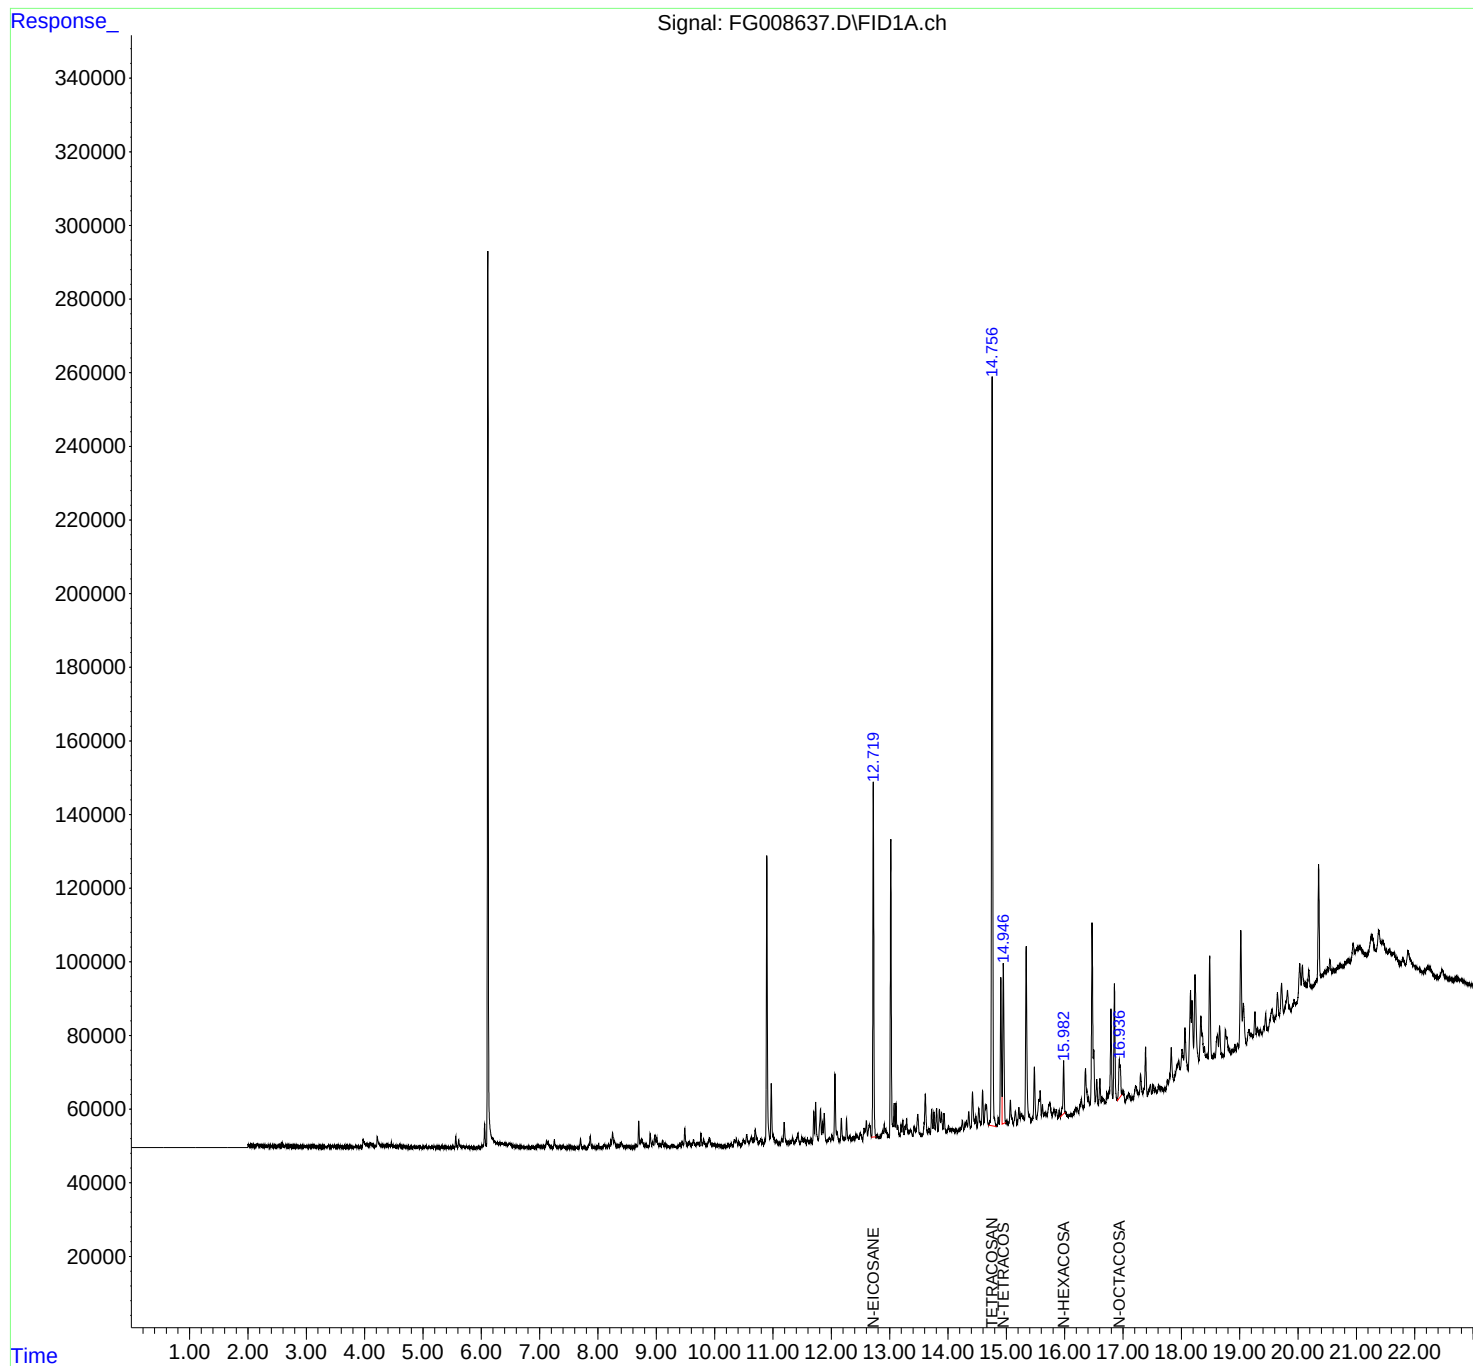


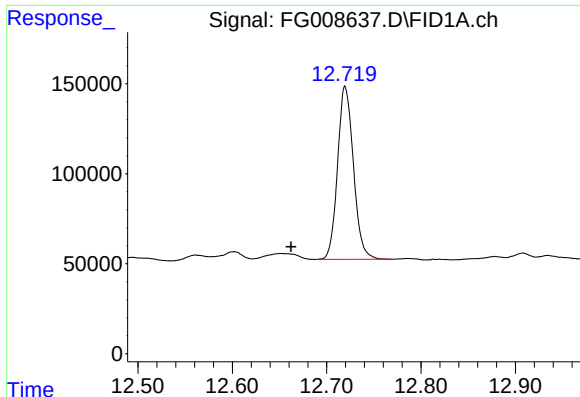

#7 N-EICOSANE


R.T.: 12.720 min
Delta R.T.: 0.057 min
Response: 1125924
Conc: 6.91 ug/ml

Instrument :
FID_G
ClientSampleId :

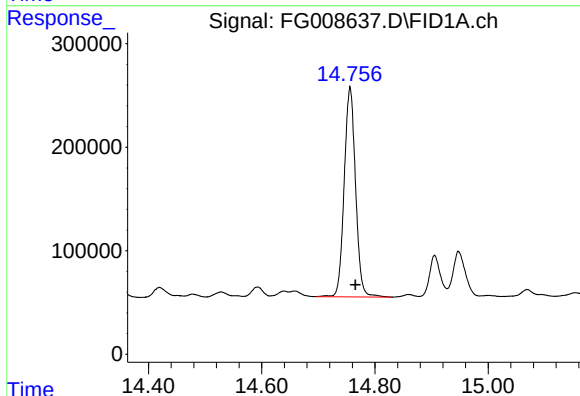


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.756 min
Delta R.T.: -0.009 min
Response: 2818075
Conc: 19.78 ug/ml

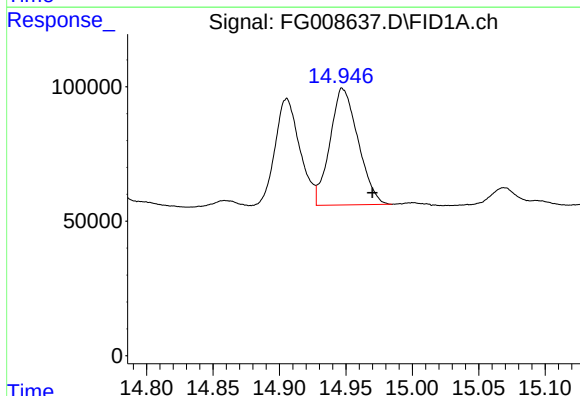


#10 N-TETRACOSANE

R.T.: 14.948 min
Delta R.T.: -0.022 min
Response: 640790
Conc: 3.91 ug/ml

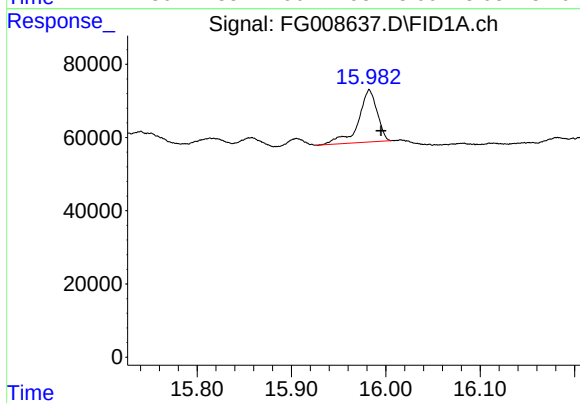

#11 N-HEXACOSANE

R.T.: 15.983 min
Delta R.T.: -0.012 min
Response: 196880
Conc: 1.21 ug/ml

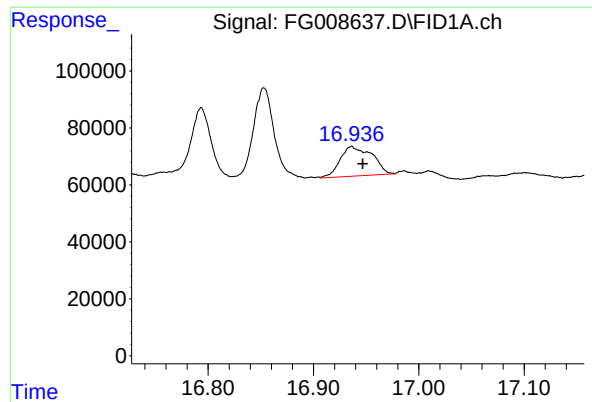

#12 N-OCTACOSANE

R.T.: 16.936 min
Delta R.T.: -0.011 min
Response: 218472
Conc: 1.36 ug/ml

Instrument :
FID_G
ClientSampleId :