

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081321\
 Data File : FG008620.D
 Signal(s) : FID1A.ch
 Acq On : 13 Aug 2021 12:03
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 50 PPM TRPH STD

Integration File: autoint1.e
 Quant Time: Aug 13 22:45:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG071521.M
 Quant Title :
 QLast Update : Thu Jul 15 13:17:03 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.760	7628658	53.538 ug/ml
Target Compounds			
2) N-DECANE	4.459	9164791	60.837 ug/ml
3) N-DODECANE	6.488	9263684	60.194 ug/ml
4) N-TETRADECANE	8.290	9337801	59.935 ug/ml
5) N-HEXADECANE	9.897	9236564	59.492 ug/ml
6) N-OCTADECANE	11.343	9360177	57.892 ug/ml
7) N-EICOSANE	12.657	9171659	56.278 ug/ml
8) N-DOCOSANE	13.858	8901513	54.625 ug/ml
10) N-TETRACOSANE	14.965	8676285	52.902 ug/ml
11) N-HEXACOSANE	15.987	8317347	51.294 ug/ml
12) N-OCTACOSANE	16.941	7989162	49.853 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081321\
Data File : FG008620.D
Signal(s) : FID1A.ch
Acq On : 13 Aug 2021 12:03
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

Integration File: autoint1.e
Quant Time: Aug 13 22:45:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG071521.M
Quant Title :
QLast Update : Thu Jul 15 13:17:03 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

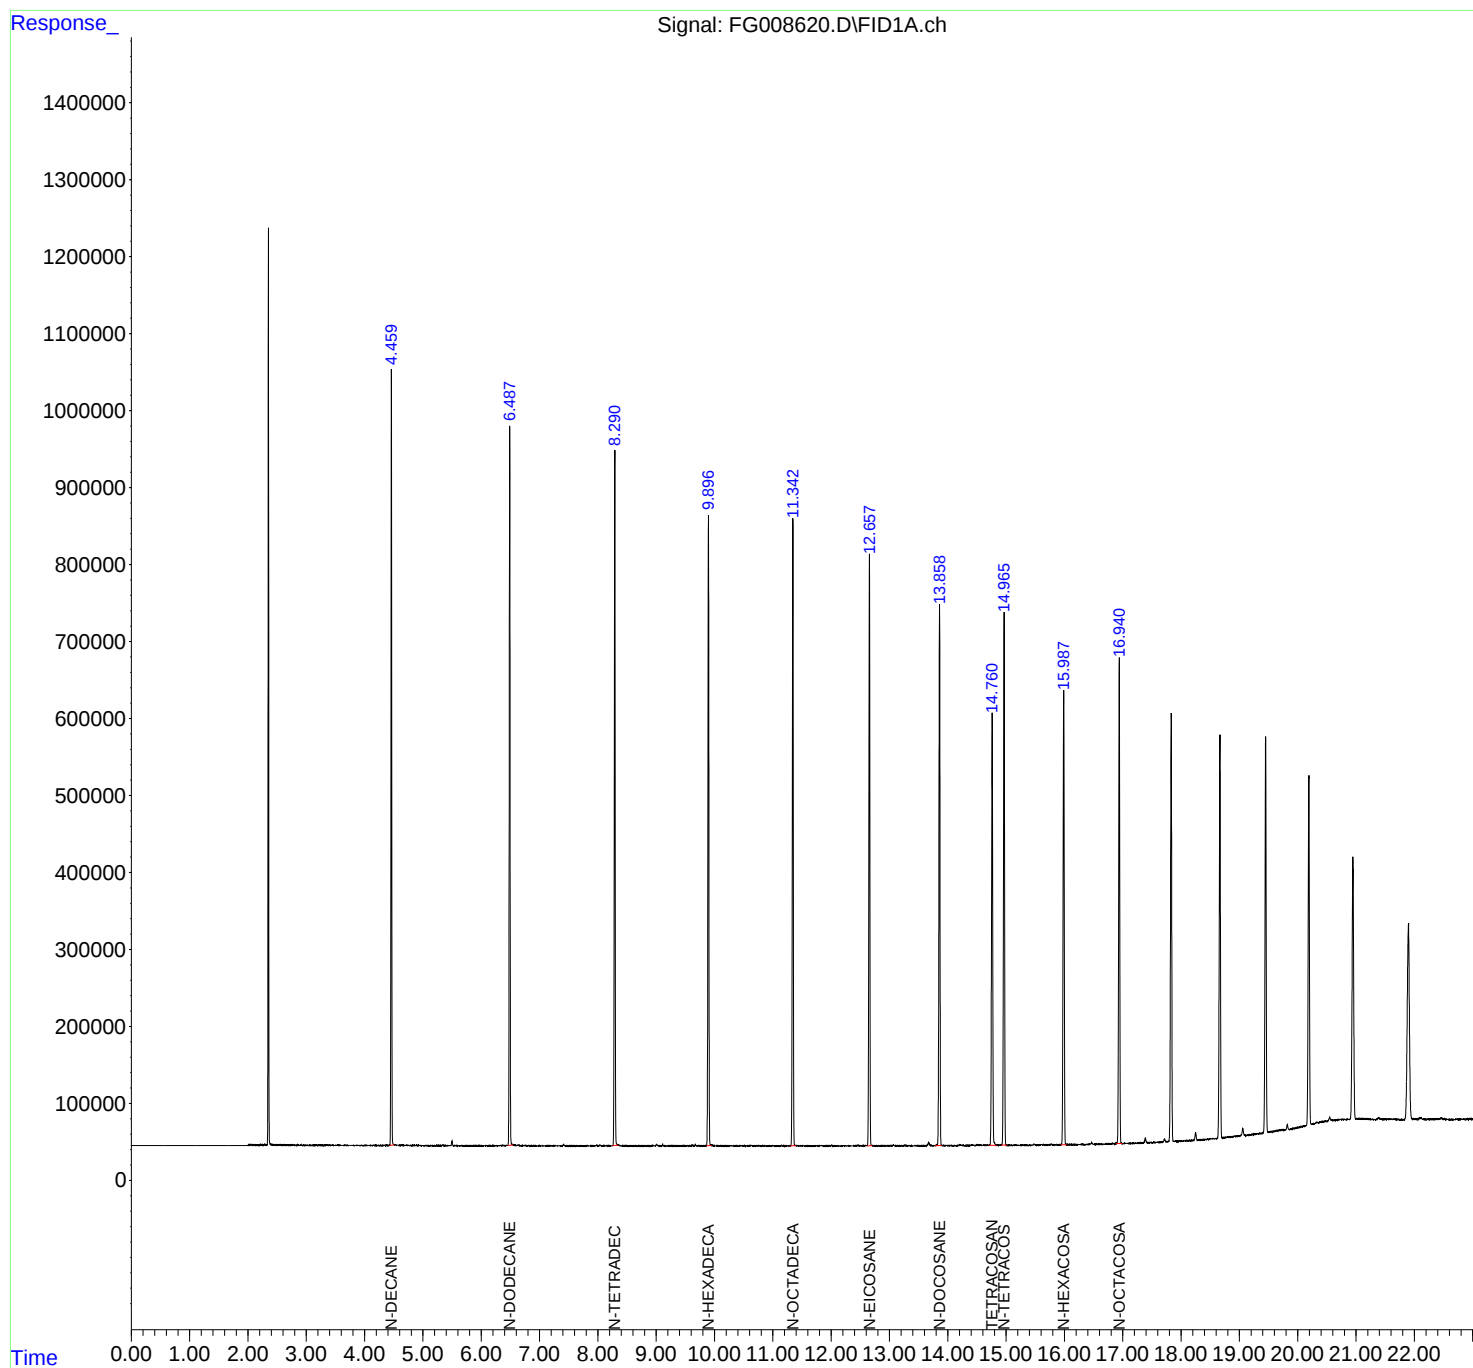


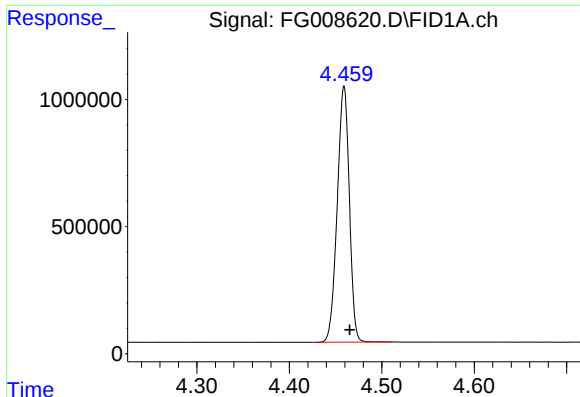

#2 N-DECANE


R.T.: 4.459 min
Delta R.T.: -0.006 min
Response: 9164791
Conc: 60.84 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

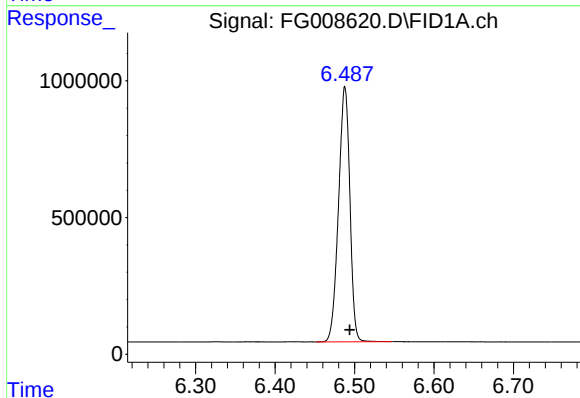


#3 N-DODECANE

R.T.: 6.488 min
Delta R.T.: -0.006 min
Response: 9263684
Conc: 60.19 ug/ml

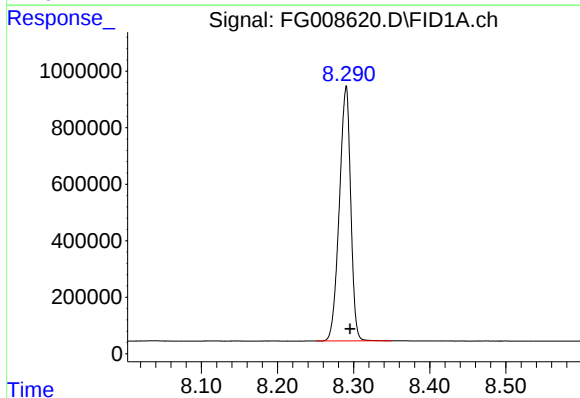


#4 N-TETRADECANE

R.T.: 8.290 min
Delta R.T.: -0.005 min
Response: 9337801
Conc: 59.93 ug/ml

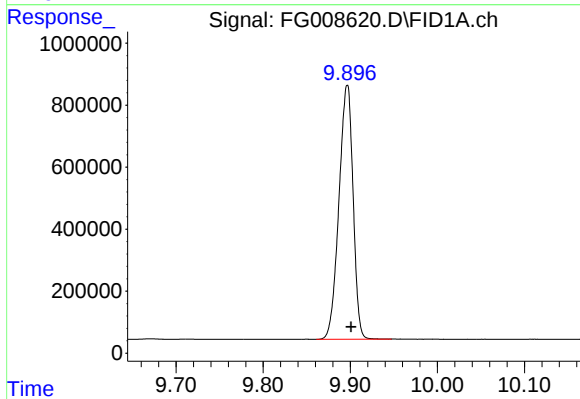

#5 N-HEXADECANE


R.T.: 9.897 min
Delta R.T.: -0.004 min
Response: 9236564
Conc: 59.49 ug/ml

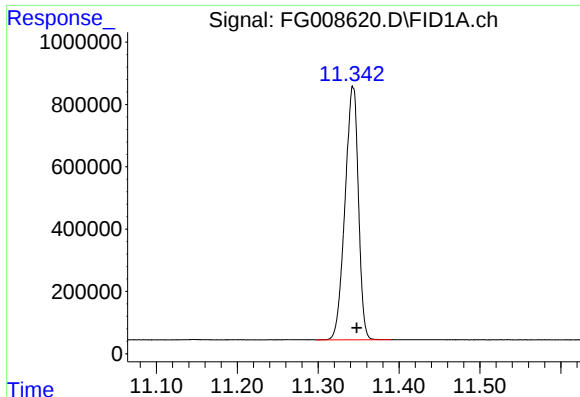

#6 N-OCTADECANE


R.T.: 11.343 min
Delta R.T.: -0.005 min
Response: 9360177
Conc: 57.89 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

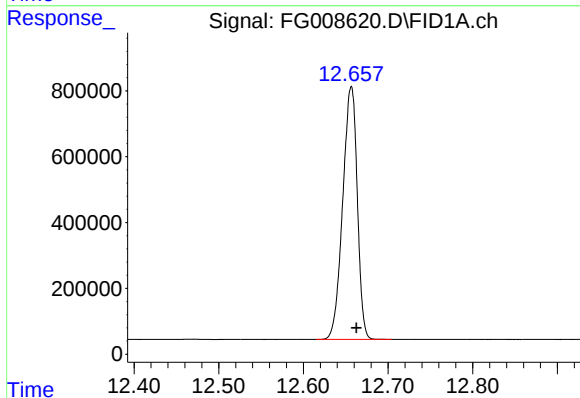


#7 N-EICOSANE

R.T.: 12.657 min
Delta R.T.: -0.006 min
Response: 9171659
Conc: 56.28 ug/ml

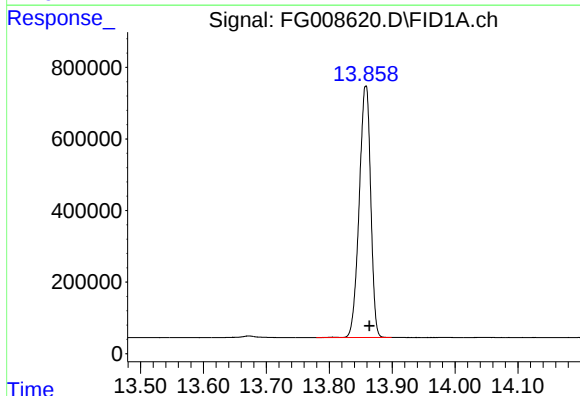


#8 N-DOCOSANE

R.T.: 13.858 min
Delta R.T.: -0.006 min
Response: 8901513
Conc: 54.63 ug/ml

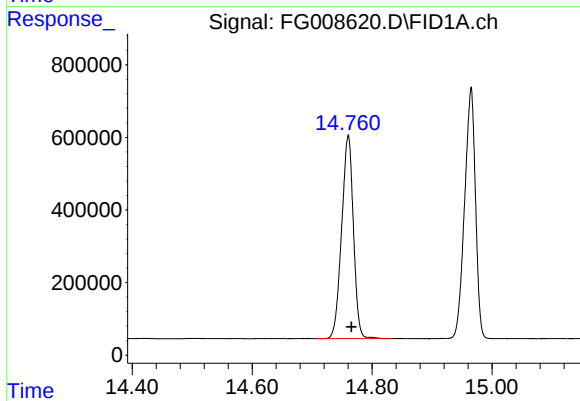

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.760 min
Delta R.T.: -0.005 min
Response: 7628658
Conc: 53.54 ug/ml

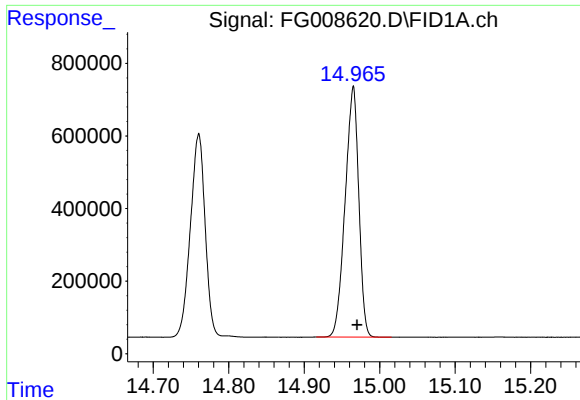

#10 N-TETRACOSANE


R.T.: 14.965 min
Delta R.T.: -0.005 min
Response: 8676285
Conc: 52.90 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

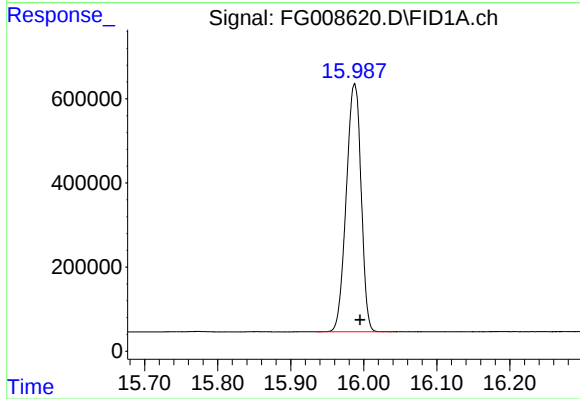

#11 N-HEXACOSANE

R.T.: 15.987 min
Delta R.T.: -0.007 min
Response: 8317347
Conc: 51.29 ug/ml

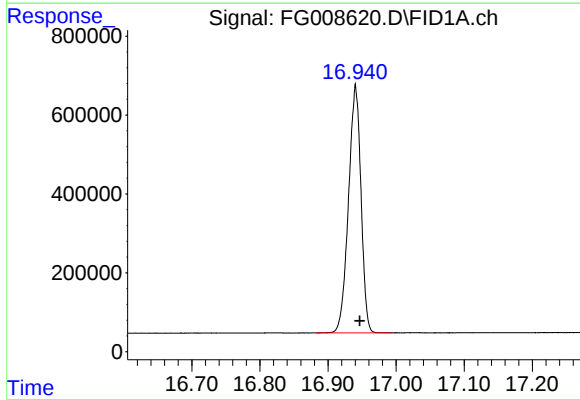

#12 N-OCTACOSANE

R.T.: 16.941 min
Delta R.T.: -0.006 min
Response: 7989162
Conc: 49.85 ug/ml