

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081423\
Data File : FG012713.D
Signal(s) : FID1A.ch
Acq On : 14 Aug 2023 19:00
Operator : YP\AJ
Sample : 03985-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PNNL-APM2-0811-2

Integration File: autoint1.e
Quant Time: Aug 15 09:01:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080223.M
Quant Title :
QLast Update : Wed Aug 02 18:57:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.083	1862899	16.653 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081423\
Data File : FG012713.D
Signal(s) : FID1A.ch
Acq On : 14 Aug 2023 19:00
Operator : YP\AJ
Sample : 03985-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PNNL-APM2-0811-2

Integration File: autoint1.e
Quant Time: Aug 15 09:01:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080223.M
Quant Title :
QLast Update : Wed Aug 02 18:57:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

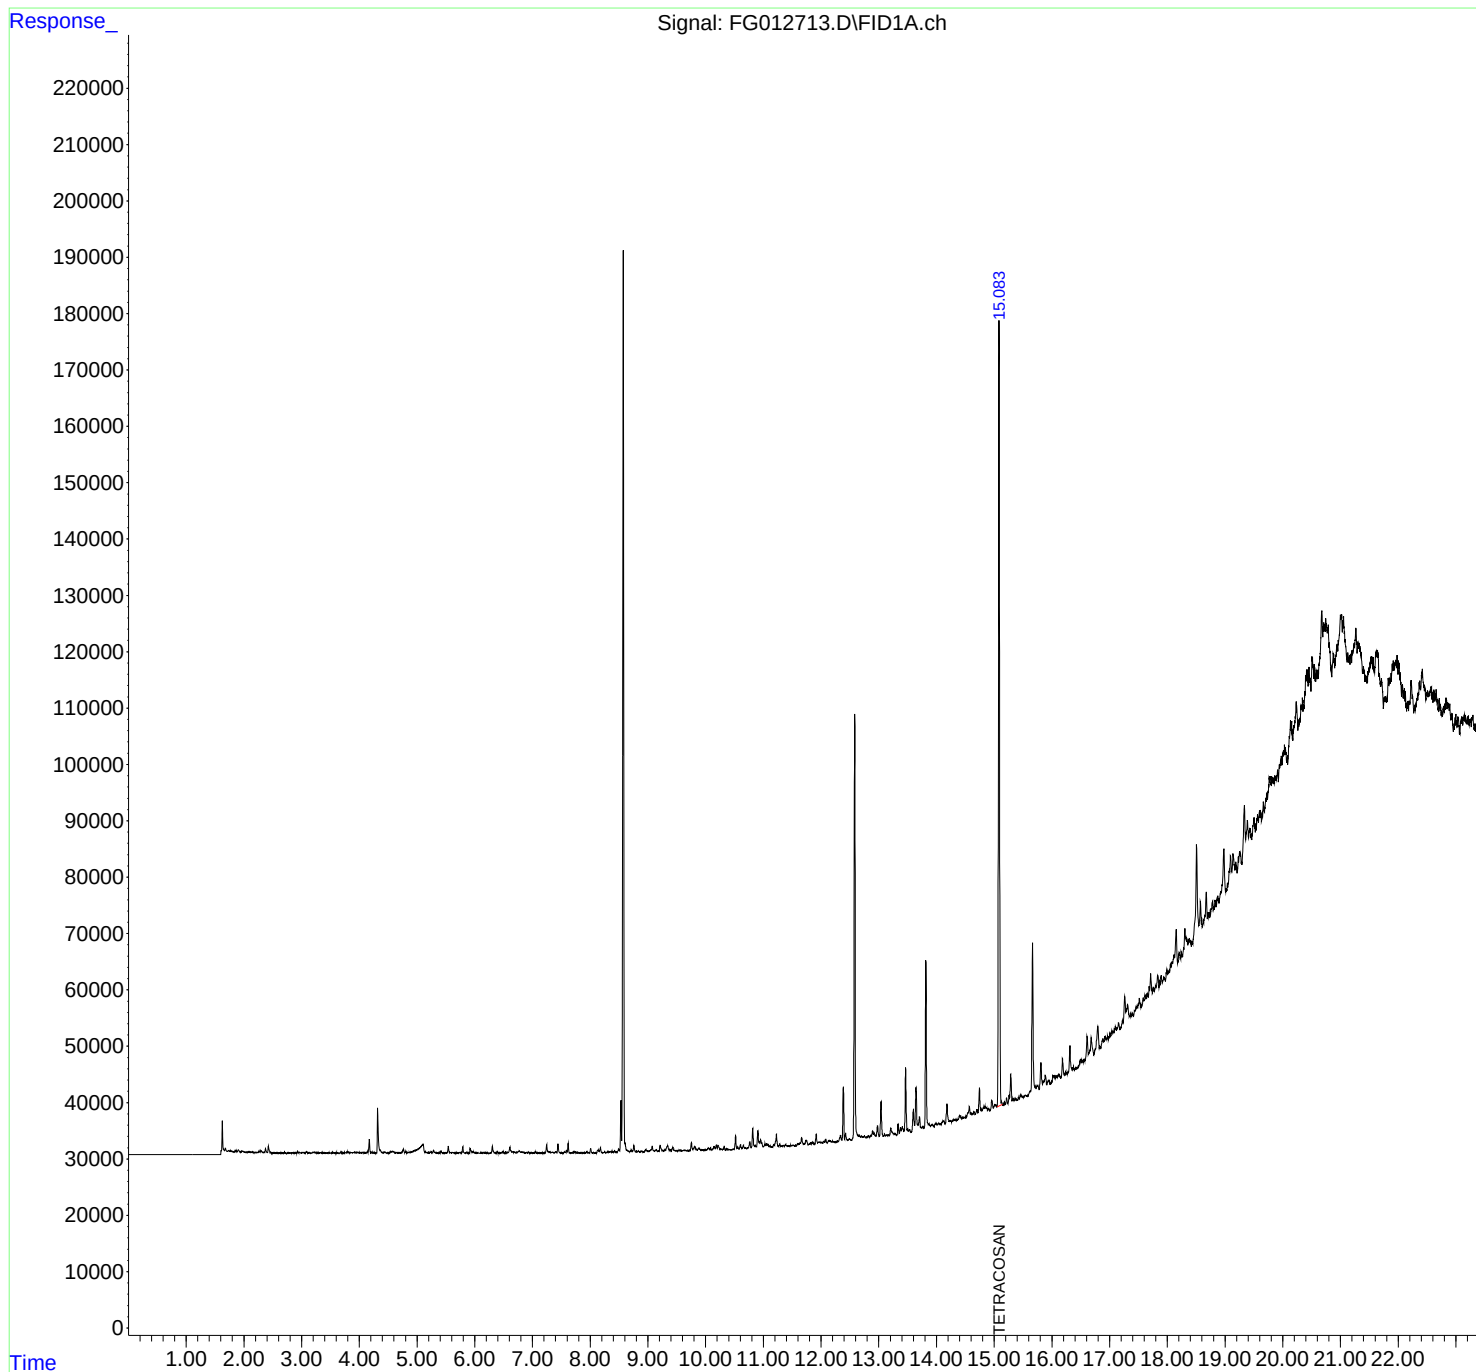

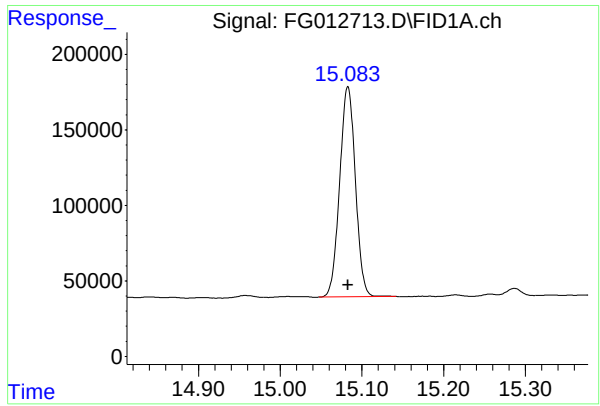

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.083 min
Delta R.T.: 0.000 min
Response: 1862899
Conc: 16.65 ug/ml

Instrument :
FID_G
ClientSampleId :
PNNL-APM2-0811-2