

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG081522\  
Data File : FG010370.D  
Signal(s) : FID1A.ch  
Acq On : 15 Aug 2022 13:59  
Operator : YP\AJ  
Sample : N4189-19  
Misc :  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :  
SB11

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 08/16/2022  
Supervised By :Ankita Jodhani 08/16/2022

Integration File: autoint1.e  
Quant Time: Aug 15 15:27:20 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG072822.M  
Quant Title :  
QLast Update : Thu Jul 28 15:10:44 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units    |
|-------------------------------|--------|----------|---------------|
| -----                         |        |          |               |
| System Monitoring Compounds   |        |          |               |
| 9) S TETRACOSANE-d50 (SURR... | 14.799 | 2068671  | 16.285 ug/mlm |
| Target Compounds              |        |          |               |
| -----                         |        |          |               |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG081522\  
Data File : FG010370.D  
Signal(s) : FID1A.ch  
Acq On : 15 Aug 2022 13:59  
Operator : YP\AJ  
Sample : N4189-19  
Misc :  
ALS Vial : 10 Sample Multiplier: 1


Instrument :  
FID\_G  
ClientSampleId :  
SB11


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 08/16/2022  
Supervised By :Ankita Jodhani 08/16/2022

Integration File: autoint1.e  
Quant Time: Aug 15 15:27:20 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG072822.M  
Quant Title :  
QLast Update : Thu Jul 28 15:10:44 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

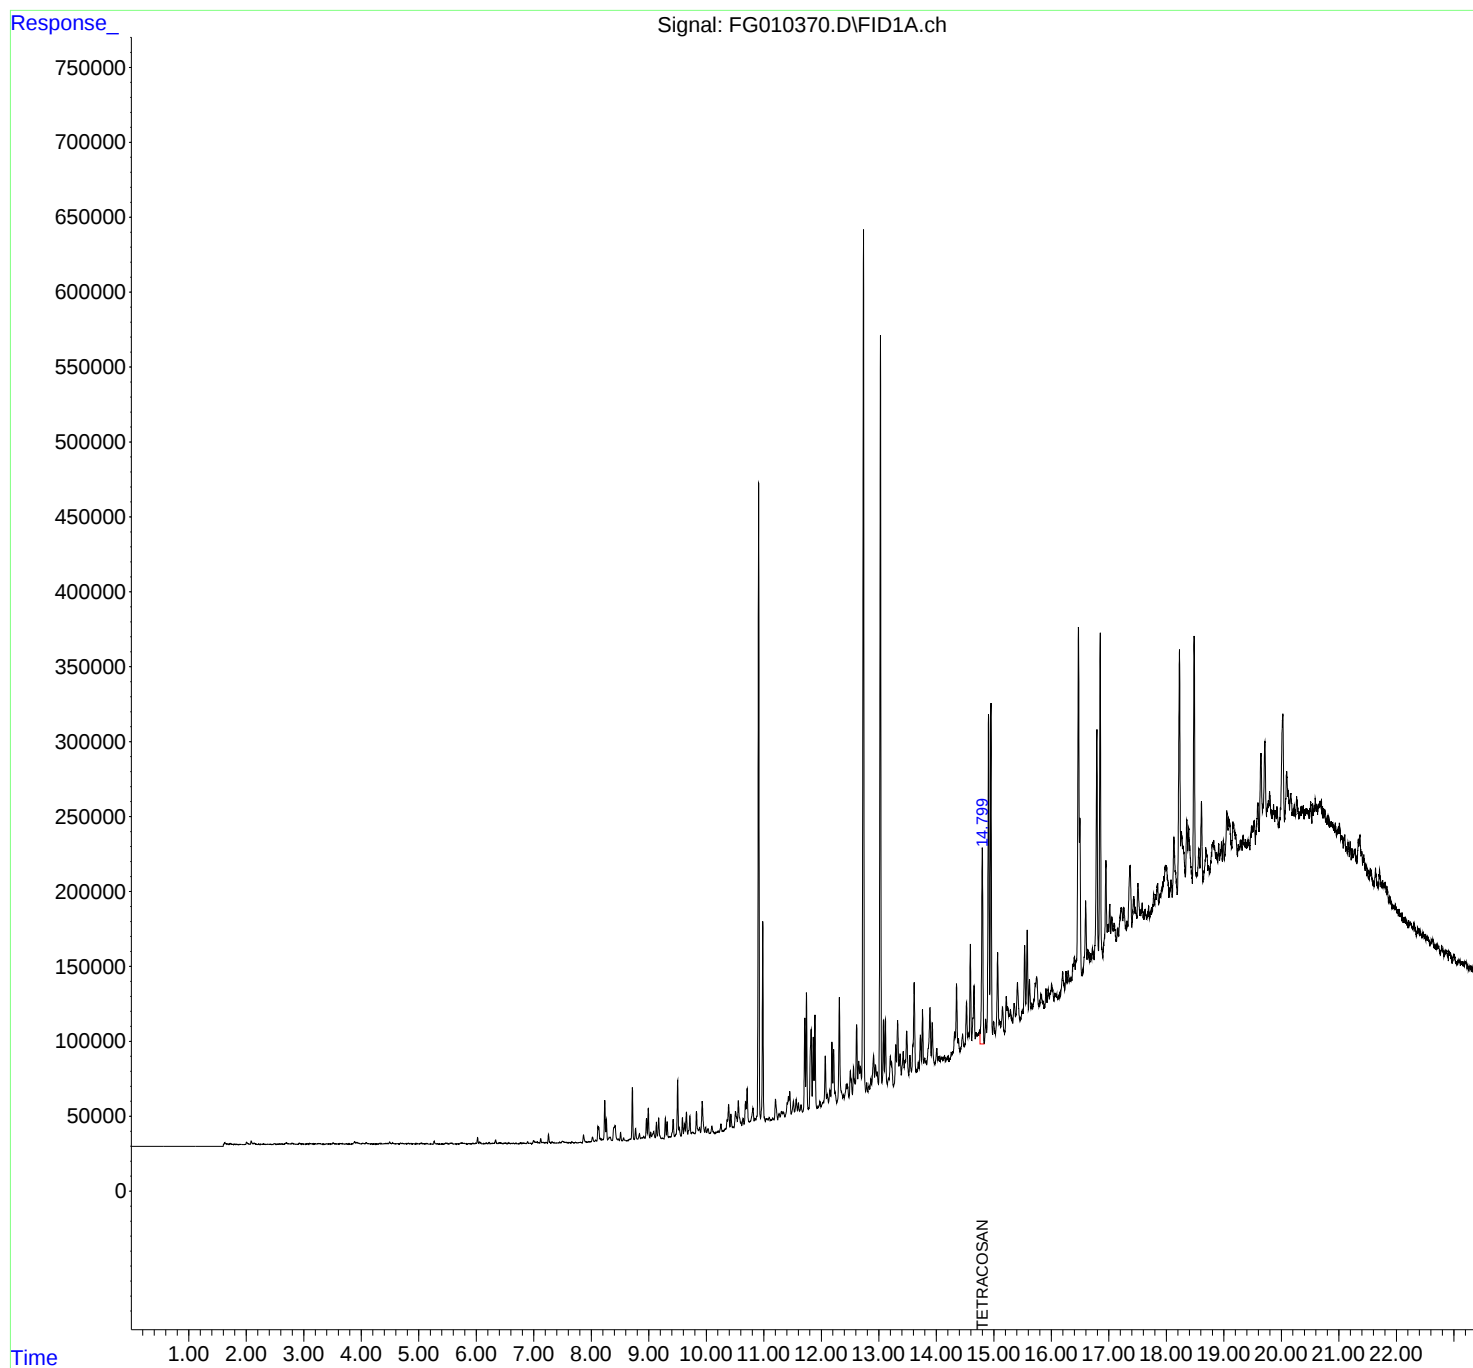

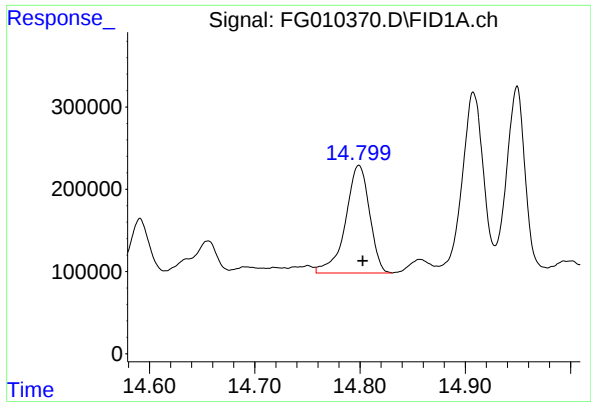

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.799 min  
Delta R.T.: -0.004 min  
Response: 2068671  
Conc: 16.28 ug/ml

Instrument :  
FID\_G  
ClientSampleId :  
SB11

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 08/16/2022  
Supervised By :Ankita Jodhani 08/16/2022