

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081718\
Data File : FG002114.D
Signal(s) : FID1A.ch
Acq On : 17 Aug 2018 17:23
Operator : AJ\SJ
Sample : J4282-07 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 18 00:45:58 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG073018.M
Quant Title :
QLast Update : Mon Jul 30 13:56:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.455	148539	1.178 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.352	118578	0.957 ug/ml
15)	N-TETRATRIACONTANE	19.139	125926	1.158 ug/ml
16)	N-HEXATRIACONTANE	19.874	43069	0.448 ug/ml
17)	N-OCTATRIACONTANE	20.593	89111	1.058 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081718\
Data File : FG002114.D
Signal(s) : FID1A.ch
Acq On : 17 Aug 2018 17:23
Operator : AJ\SJ
Sample : J4282-07 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 18 00:45:58 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG073018.M
Quant Title :
QLast Update : Mon Jul 30 13:56:56 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

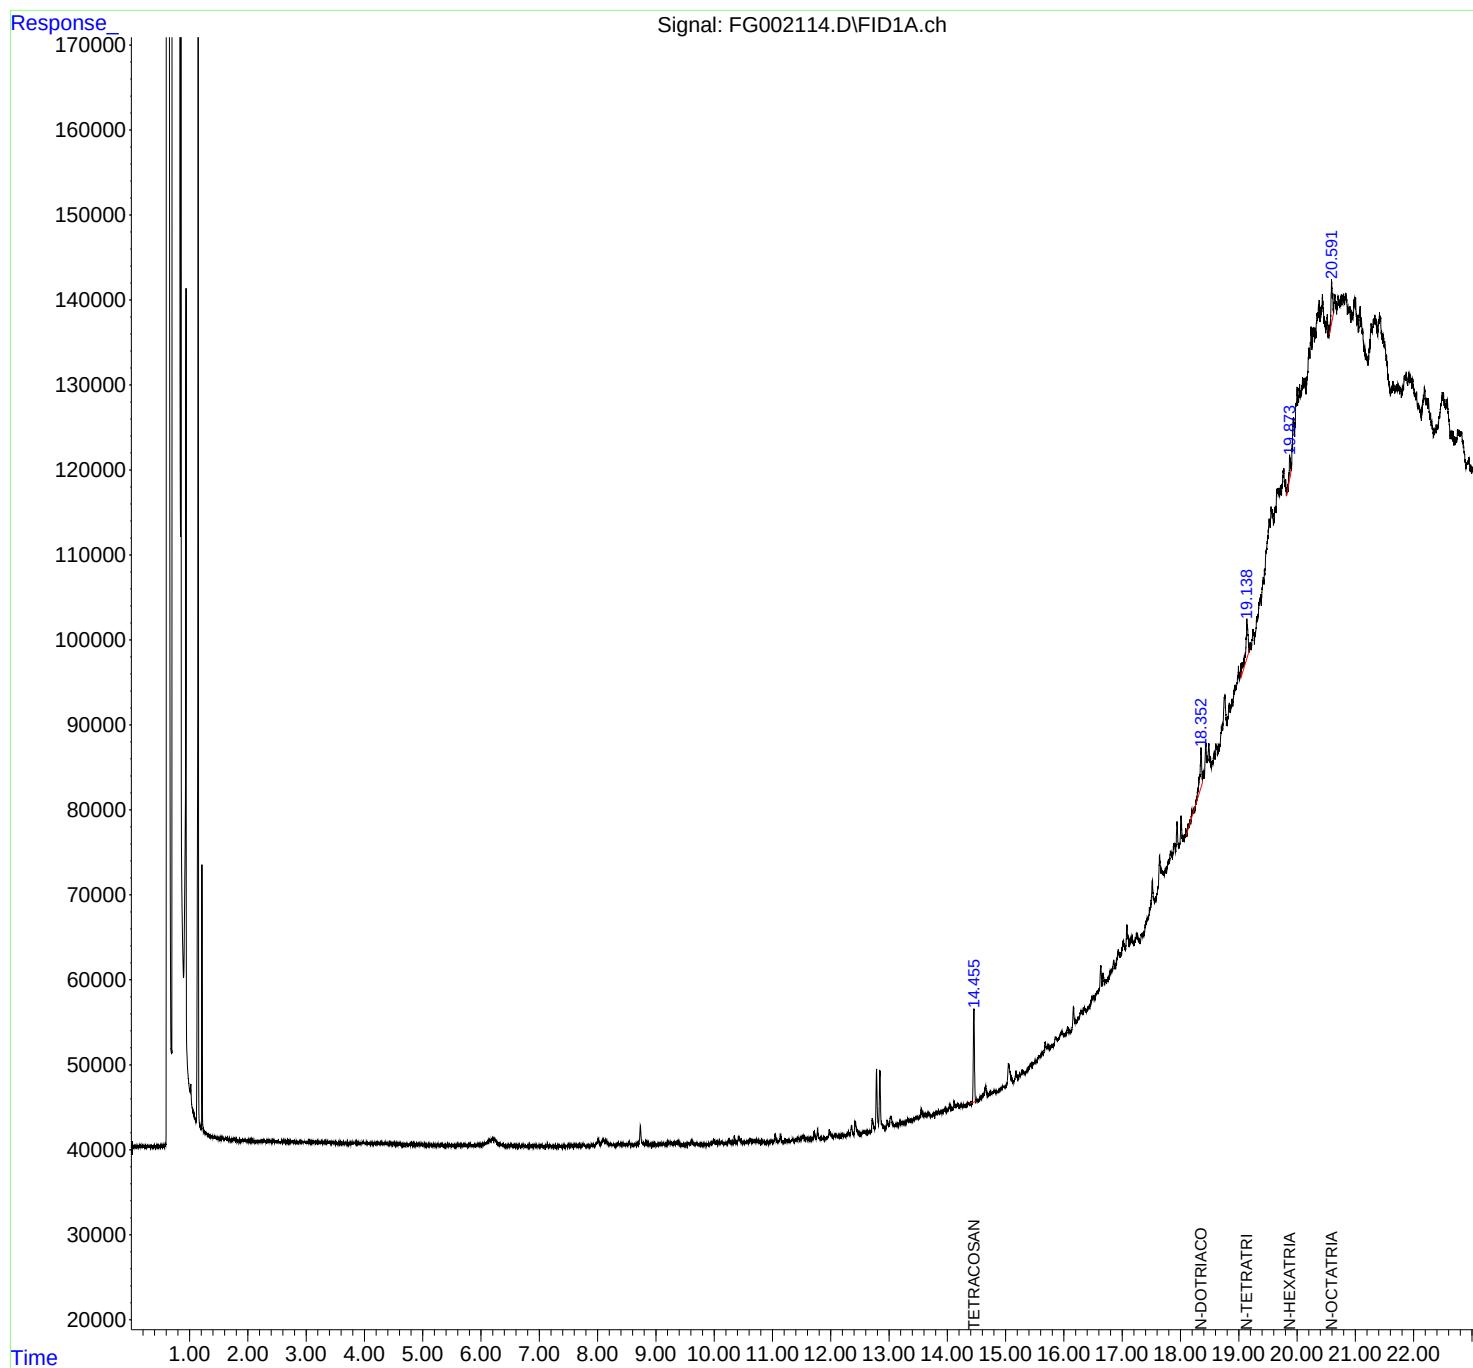

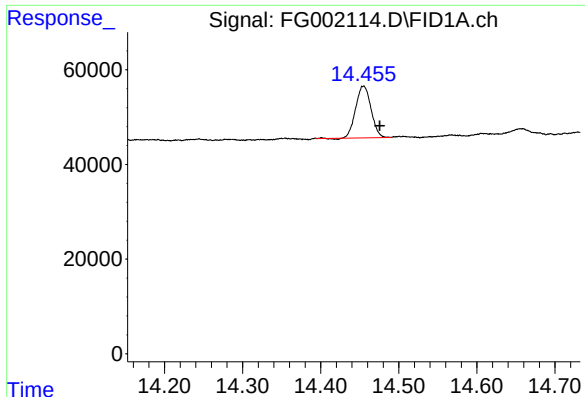


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.455 min
Delta R.T.: -0.021 min
Response: 148539
Conc: 1.18 ug/ml

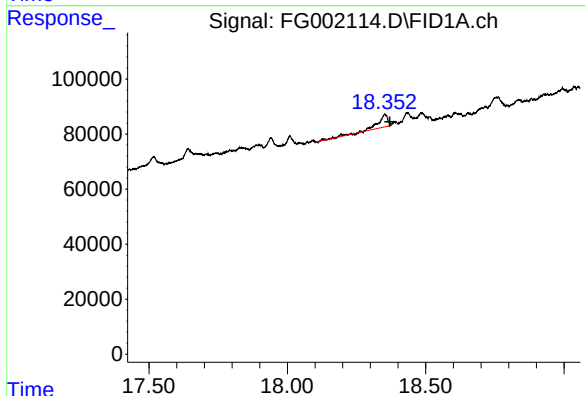


#14 N-DOTRIACONTANE

R.T.: 18.352 min
Delta R.T.: -0.018 min
Response: 118578
Conc: 0.96 ug/ml

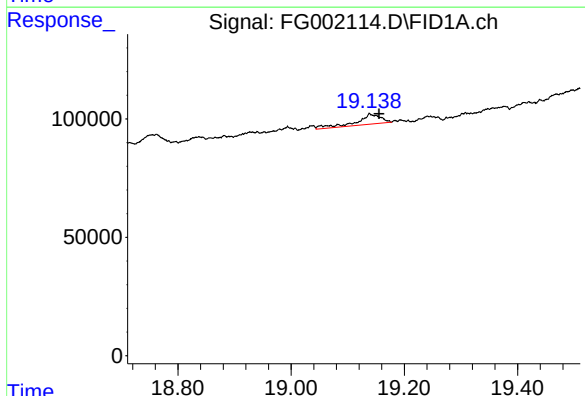


#15 N-TETRATRIACONTANE

R.T.: 19.139 min
Delta R.T.: -0.016 min
Response: 125926
Conc: 1.16 ug/ml

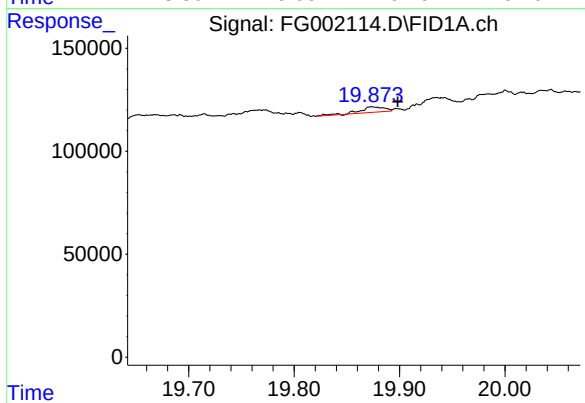

#16 N-HEXATRIACONTANE

R.T.: 19.874 min
Delta R.T.: -0.025 min
Response: 43069
Conc: 0.45 ug/ml

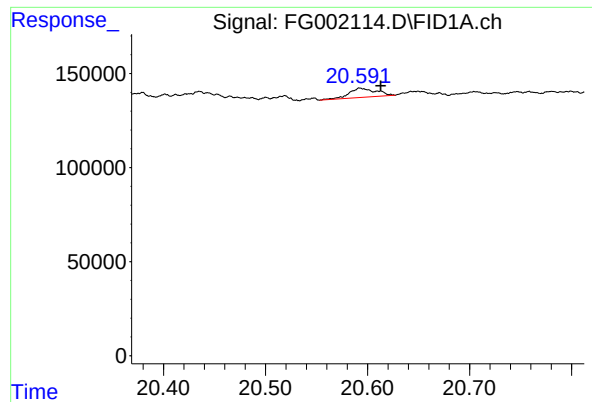

#17 N-OCTATRIACONTANE

R.T.: 20.593 min
Delta R.T.: -0.020 min
Response: 89111
Conc: 1.06 ug/ml