

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081721\
 Data File : FG008691.D
 Signal(s) : FID1A.ch
 Acq On : 17 Aug 2021 09:26
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Aug 17 14:37:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG081621.M
 Quant Title :
 QLast Update : Tue Aug 17 02:29:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.755	4996604	41.617 ug/ml
Target Compounds			
2) N-DECANE	4.457	6542558	44.055 ug/ml
3) N-DODECANE	6.484	6538132	43.377 ug/ml
4) N-TETRADECANE	8.285	6467446	42.746 ug/ml
5) N-HEXADECANE	9.890	6320601	42.346 ug/ml
6) N-OCTADECANE	11.337	6233619	41.667 ug/ml
7) N-EICOSANE	12.651	6182511	41.388 ug/ml
8) N-DOCOSANE	13.853	5994696	41.309 ug/ml
10) N-TETRACOSANE	14.960	5741140	41.298 ug/ml
11) N-HEXACOSANE	15.982	5506488	41.695 ug/ml
12) N-OCTACOSANE	16.934	5308679	42.422 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081721\
Data File : FG008691.D
Signal(s) : FID1A.ch
Acq On : 17 Aug 2021 09:26
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 17 14:37:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG081621.M
Quant Title :
QLast Update : Tue Aug 17 02:29:16 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

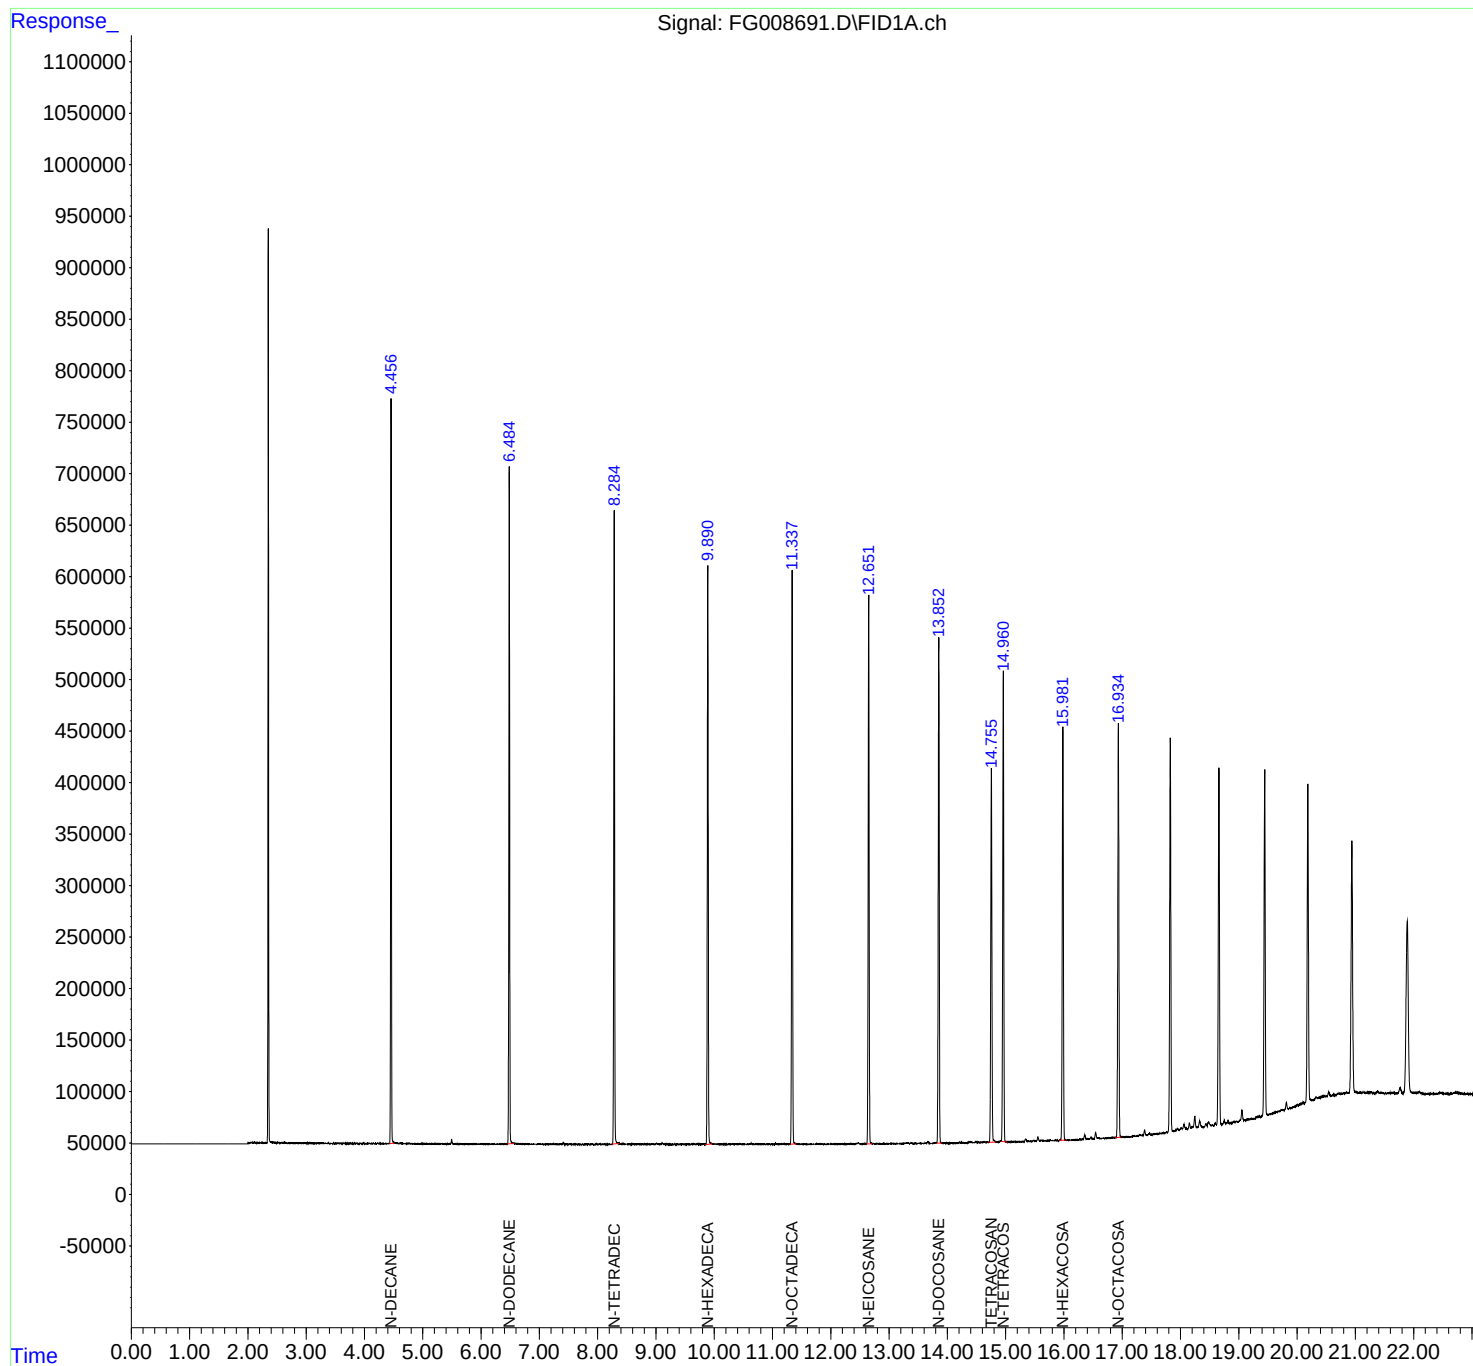

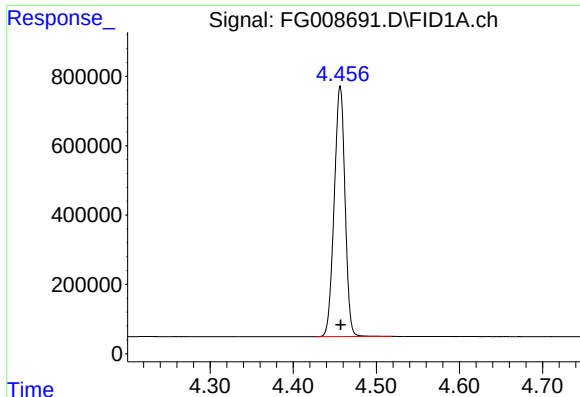


#2 N-DECANE

R.T.: 4.457 min
Delta R.T.: 0.000 min
Response: 6542558
Conc: 44.06 ug/ml

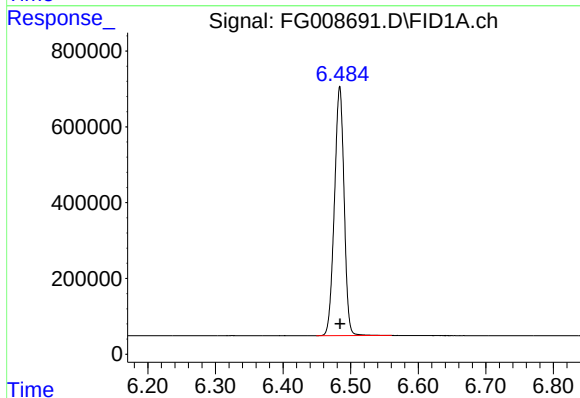


#3 N-DODECANE

R.T.: 6.484 min
Delta R.T.: 0.000 min
Response: 6538132
Conc: 43.38 ug/ml

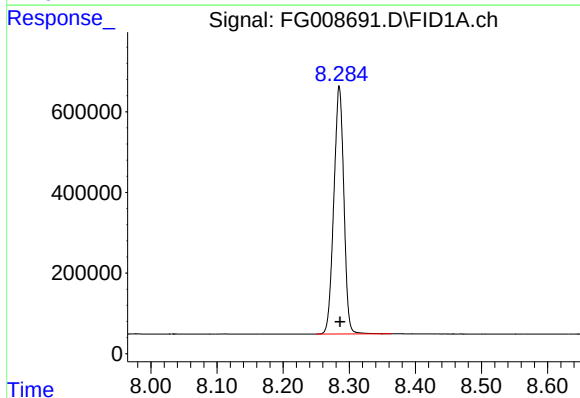


#4 N-TETRADECANE

R.T.: 8.285 min
Delta R.T.: -0.001 min
Response: 6467446
Conc: 42.75 ug/ml

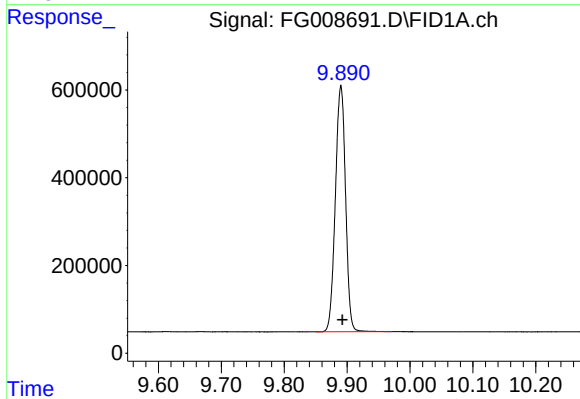


#5 N-HEXADECANE

R.T.: 9.890 min
Delta R.T.: -0.002 min
Response: 6320601
Conc: 42.35 ug/ml

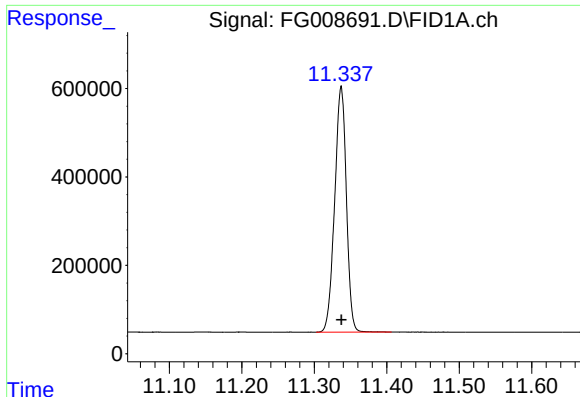


#6 N-OCTADECANE

R.T.: 11.337 min
Delta R.T.: 0.000 min
Response: 6233619
Conc: 41.67 ug/ml

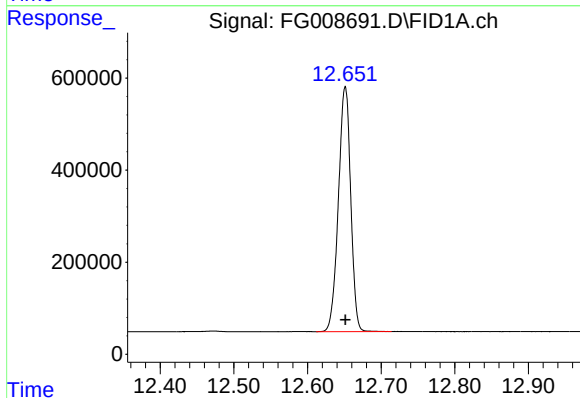


#7 N-EICOSANE

R.T.: 12.651 min
Delta R.T.: 0.000 min
Response: 6182511
Conc: 41.39 ug/ml

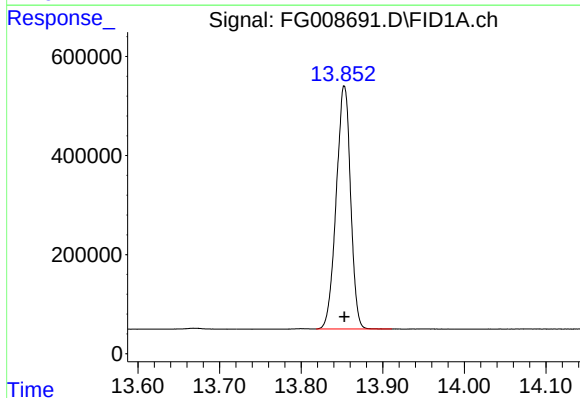


#8 N-DOCOSANE

R.T.: 13.853 min
Delta R.T.: 0.000 min
Response: 5994696
Conc: 41.31 ug/ml

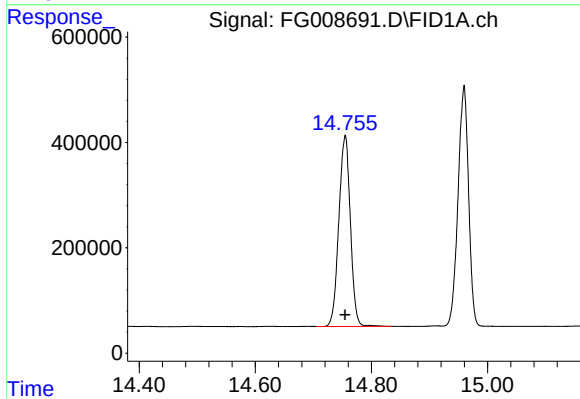


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.755 min
Delta R.T.: 0.000 min
Response: 4996604
Conc: 41.62 ug/ml

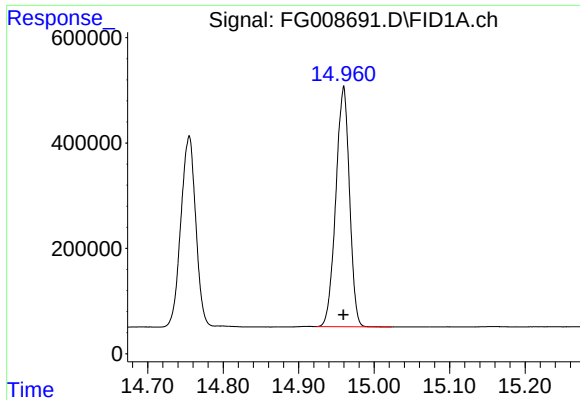


#10 N-TETRACOSANE

R.T.: 14.960 min
Delta R.T.: 0.000 min
Response: 5741140
Conc: 41.30 ug/ml

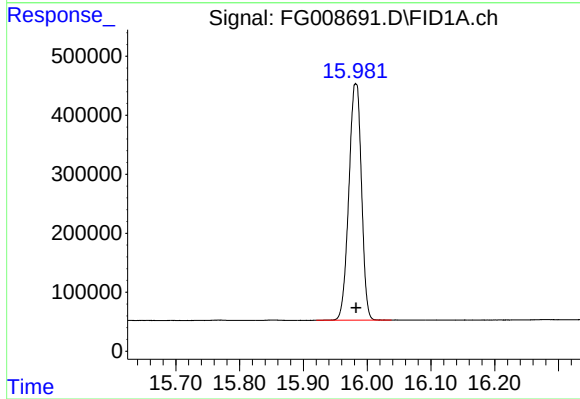

#11 N-HEXACOSANE

R.T.: 15.982 min
Delta R.T.: 0.000 min
Response: 5506488
Conc: 41.70 ug/ml

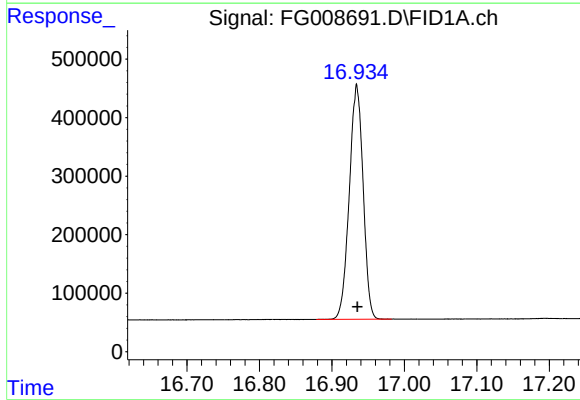

#12 N-OCTACOSANE

R.T.: 16.934 min
Delta R.T.: -0.001 min
Response: 5308679
Conc: 42.42 ug/ml