

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081821\
 Data File : FG008709.D
 Signal(s) : FID1A.ch
 Acq On : 18 Aug 2021 15:08
 Operator : DD\AJ
 Sample : PB138532BS
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 19 04:06:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG081621.M
 Quant Title :
 QLast Update : Tue Aug 17 02:29:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.749	2741354	22.833 ug/ml
Target Compounds			
2) N-DECANE	4.452	3547390	23.887 ug/ml
3) N-DODECANE	6.479	3595545	23.854 ug/ml
4) N-TETRADECANE	8.280	3579966	23.662 ug/ml
5) N-HEXADECANE	9.885	3503691	23.474 ug/ml
6) N-OCTADECANE	11.332	3484668	23.292 ug/ml
7) N-EICOSANE	12.645	3462397	23.178 ug/ml
8) N-DOCOSANE	13.847	3350146	23.085 ug/ml
10) N-TETRACOSANE	14.954	3209595	23.088 ug/ml
11) N-HEXACOSANE	15.978	3039834	23.018 ug/ml
12) N-OCTACOSANE	16.931	2907341	23.233 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081821\
Data File : FG008709.D
Signal(s) : FID1A.ch
Acq On : 18 Aug 2021 15:08
Operator : DD\AJ
Sample : PB138532BS
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 19 04:06:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG081621.M
Quant Title :
QLast Update : Tue Aug 17 02:29:16 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

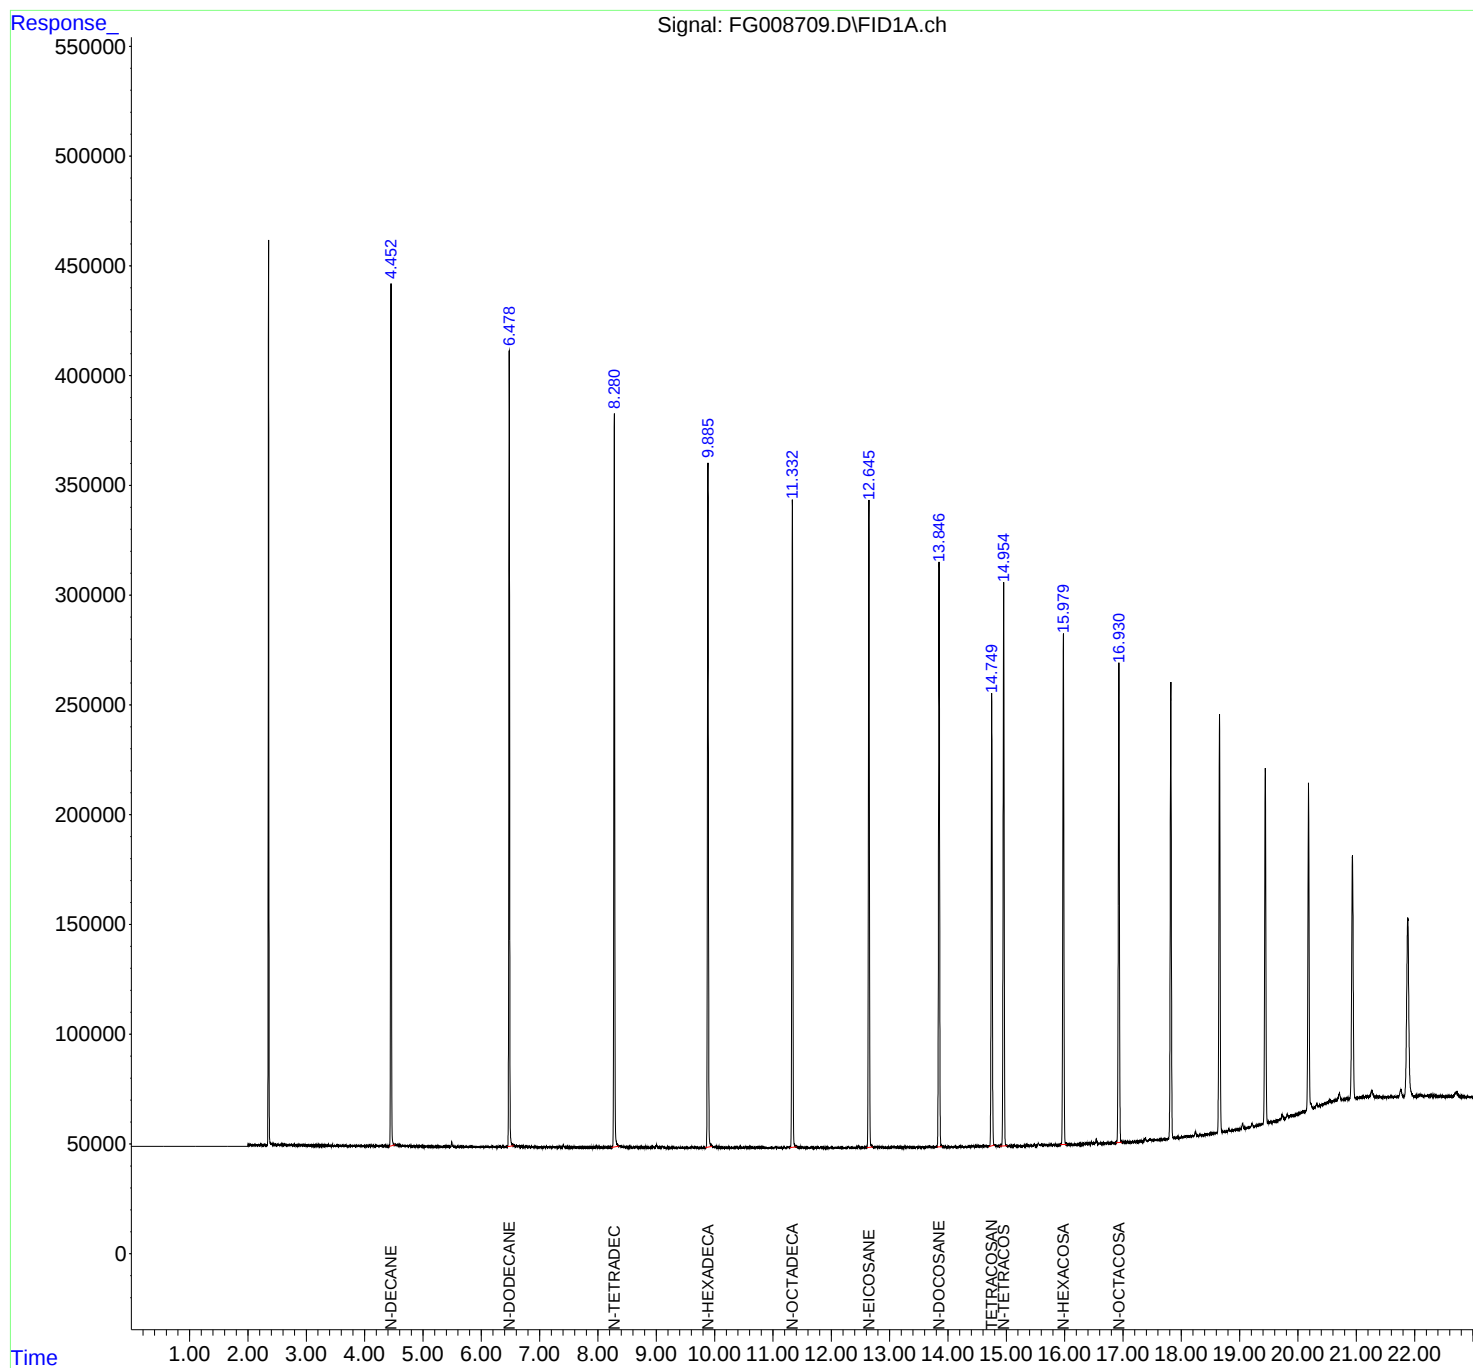


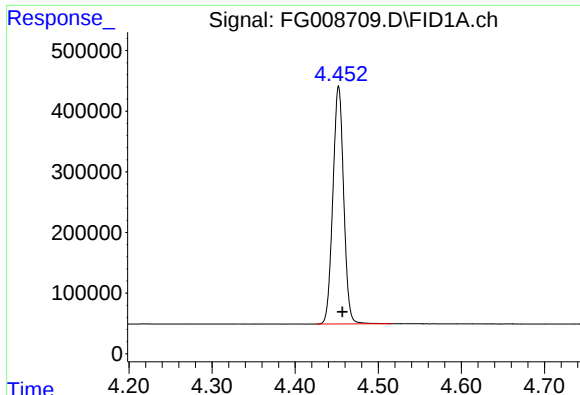

#2 N-DECANE


R.T.: 4.452 min
Delta R.T.: -0.005 min
Response: 3547390
Conc: 23.89 ug/ml

Instrument :
FID_G
ClientSampleId :

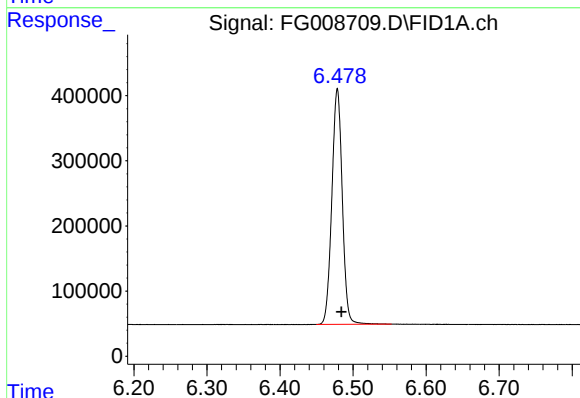


#3 N-DODECANE

R.T.: 6.479 min
Delta R.T.: -0.006 min
Response: 3595545
Conc: 23.85 ug/ml

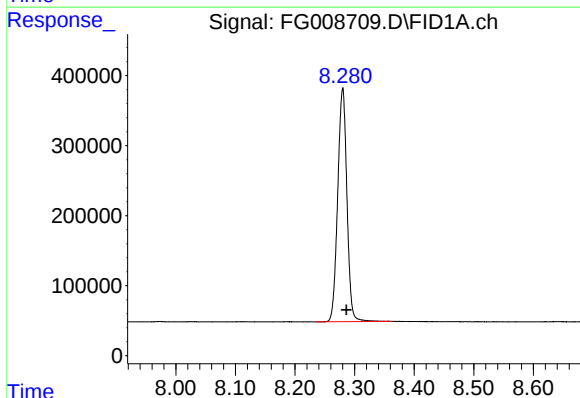


#4 N-TETRADECANE

R.T.: 8.280 min
Delta R.T.: -0.006 min
Response: 3579966
Conc: 23.66 ug/ml

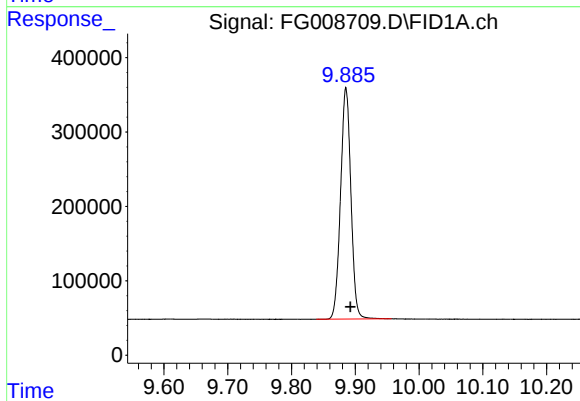

#5 N-HEXADECANE


R.T.: 9.885 min
Delta R.T.: -0.007 min
Response: 3503691
Conc: 23.47 ug/ml

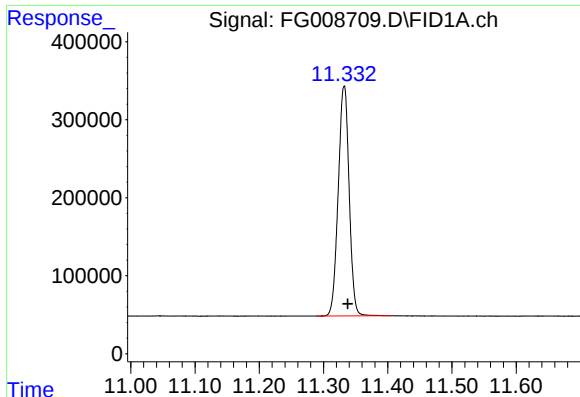

#6 N-OCTADECANE


R.T.: 11.332 min
Delta R.T.: -0.005 min
Response: 3484668
Conc: 23.29 ug/ml

Instrument :
FID_G
ClientSampleId :

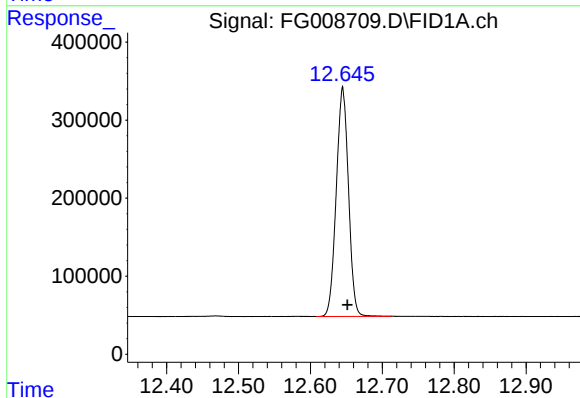


#7 N-EICOSANE

R.T.: 12.645 min
Delta R.T.: -0.007 min
Response: 3462397
Conc: 23.18 ug/ml

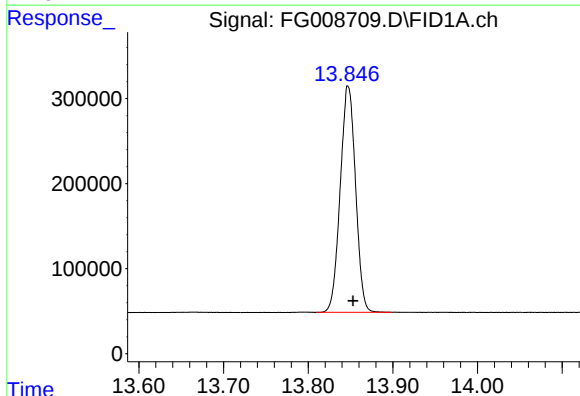


#8 N-DOCOSANE

R.T.: 13.847 min
Delta R.T.: -0.006 min
Response: 3350146
Conc: 23.09 ug/ml

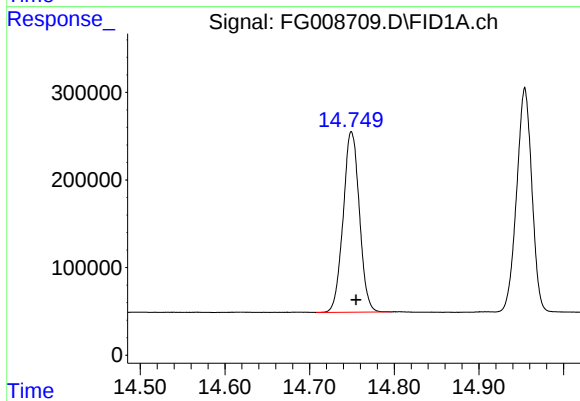

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.749 min
Delta R.T.: -0.005 min
Response: 2741354
Conc: 22.83 ug/ml

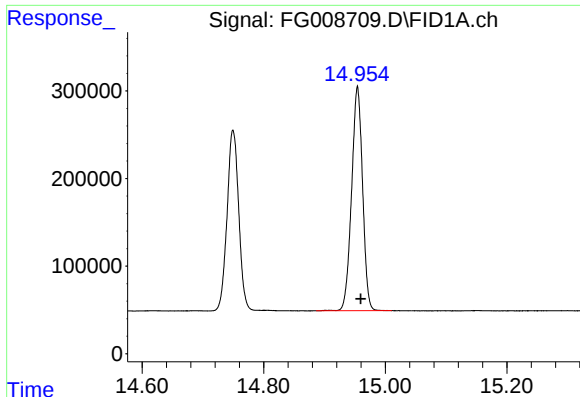

#10 N-TETRACOSANE


R.T.: 14.954 min
Delta R.T.: -0.005 min
Response: 3209595
Conc: 23.09 ug/ml

Instrument :
FID_G
ClientSampleId :

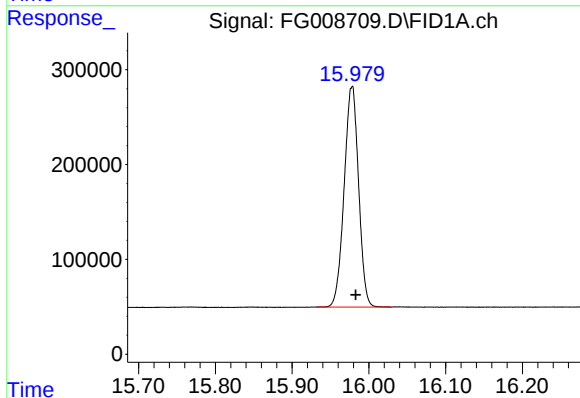

#11 N-HEXACOSANE

R.T.: 15.978 min
Delta R.T.: -0.005 min
Response: 3039834
Conc: 23.02 ug/ml

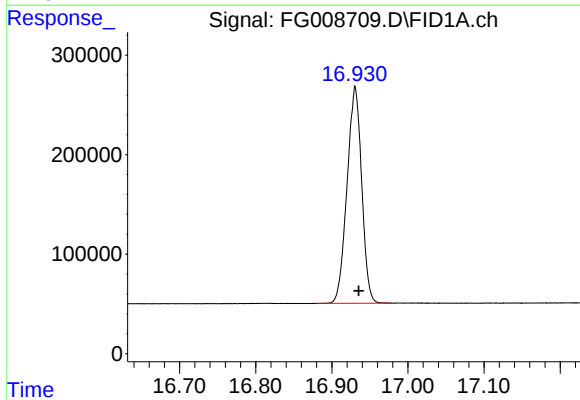

#12 N-OCTACOSANE

R.T.: 16.931 min
Delta R.T.: -0.005 min
Response: 2907341
Conc: 23.23 ug/ml