

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081821\
Data File : FG008708.D
Signal(s) : FID1A.ch
Acq On : 18 Aug 2021 14:37
Operator : DD\AJ
Sample : PB138532BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB138532BL

Integration File: autoint1.e
Quant Time: Aug 19 04:05:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG081621.M
Quant Title :
QLast Update : Tue Aug 17 02:29:16 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.750	2462568	20.511 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081821\
Data File : FG008708.D
Signal(s) : FID1A.ch
Acq On : 18 Aug 2021 14:37
Operator : DD\AJ
Sample : PB138532BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB138532BL

Integration File: autoint1.e
Quant Time: Aug 19 04:05:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG081621.M
Quant Title :
QLast Update : Tue Aug 17 02:29:16 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

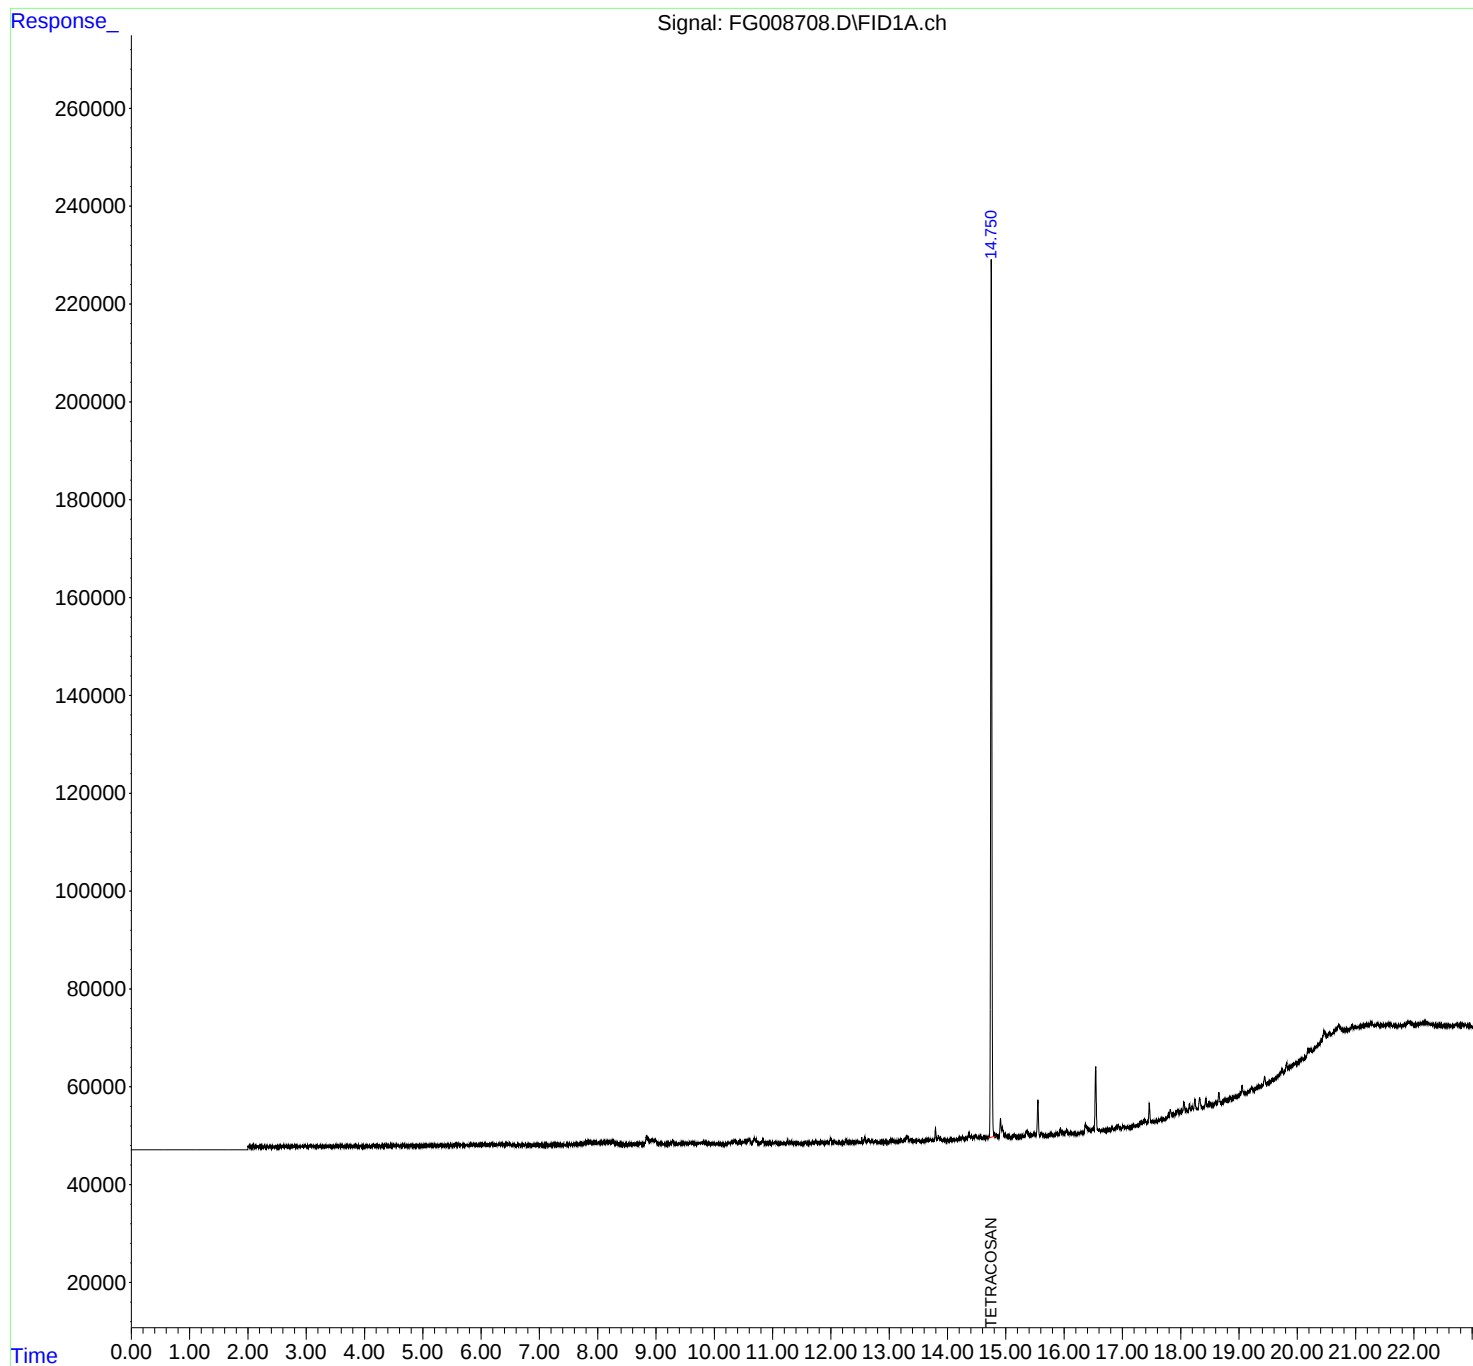

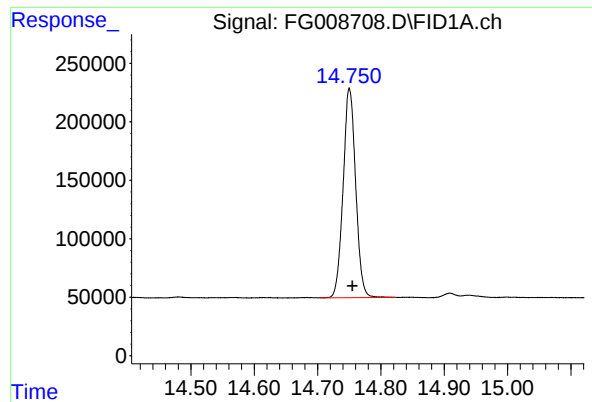

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.750 min
Delta R.T.: -0.005 min
Response: 2462568
Conc: 20.51 ug/ml

Instrument :
FID_G
ClientSampleId :
PB138532BL