

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081823\
 Data File : FG012730.D
 Signal(s) : FID1A.ch
 Acq On : 18 Aug 2023 18:55
 Operator : YP\AJ
 Sample : 04046-02 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 18 23:41:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080223.M
 Quant Title :
 QLast Update : Wed Aug 02 18:57:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.086	122632	1.096 ug/ml
Target Compounds			
7) N-EICOSANE	13.041f	104881	0.815 ug/ml
10) N-TETRACOSANE	15.265	108833	0.861 ug/ml
15) N-TETRATRIACONTANE	19.778	109013	1.151 ug/ml
16) N-HEXATRIACONTANE	20.505	72224	0.890 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081823\
Data File : FG012730.D
Signal(s) : FID1A.ch
Acq On : 18 Aug 2023 18:55
Operator : YP\AJ
Sample : 04046-02 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 18 23:41:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080223.M
Quant Title :
QLast Update : Wed Aug 02 18:57:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

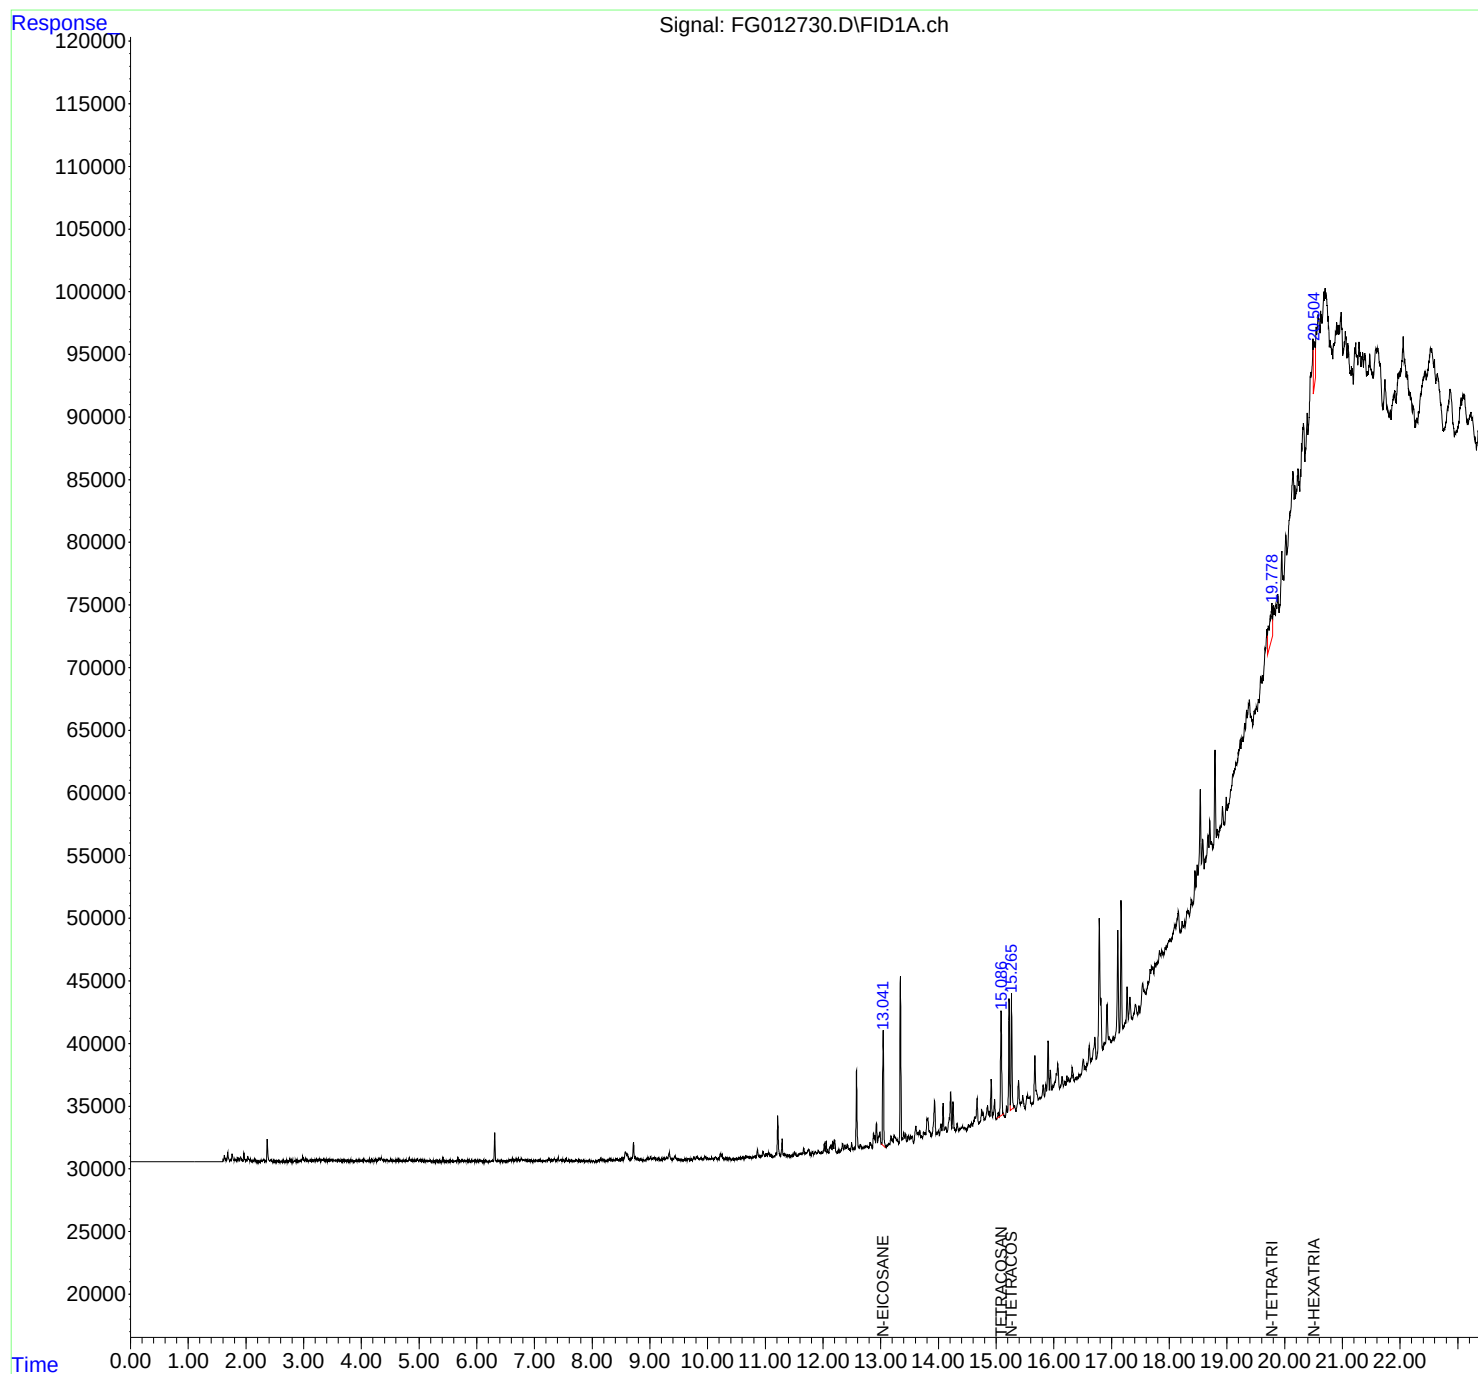


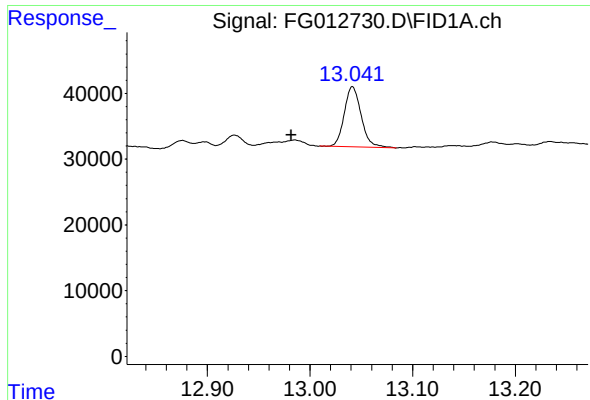

#7 N-EICOSANE


R.T.: 13.041 min
Delta R.T.: 0.060 min
Response: 104881
Conc: 0.82 ug/ml

Instrument :
FID_G
ClientSampleId :

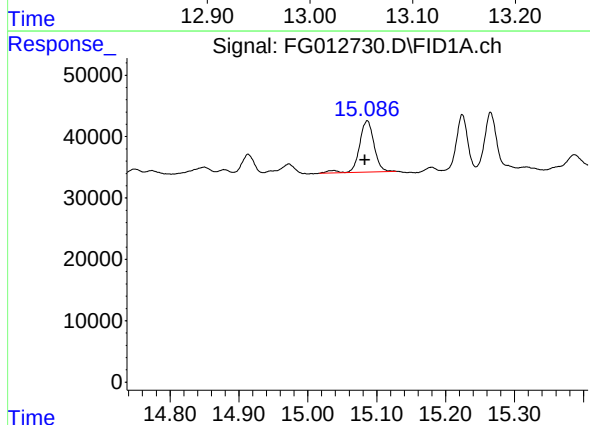


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.086 min
Delta R.T.: 0.004 min
Response: 122632
Conc: 1.10 ug/ml

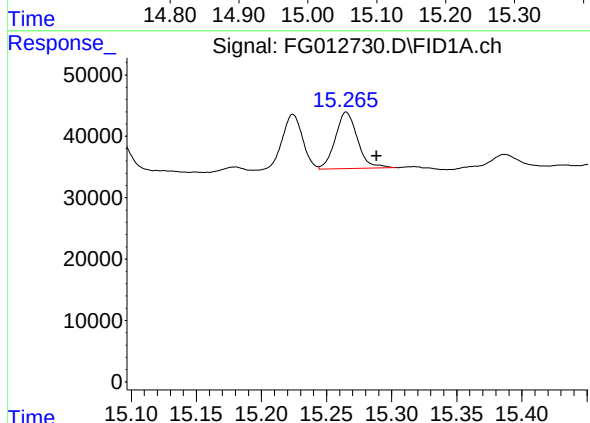


#10 N-TETRACOSANE

R.T.: 15.265 min
Delta R.T.: -0.023 min
Response: 108833
Conc: 0.86 ug/ml

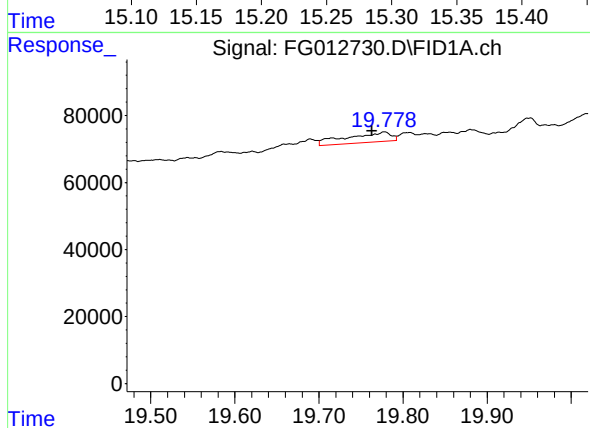

#15 N-TETRATRIACONTANE

R.T.: 19.778 min
Delta R.T.: 0.015 min
Response: 109013
Conc: 1.15 ug/ml

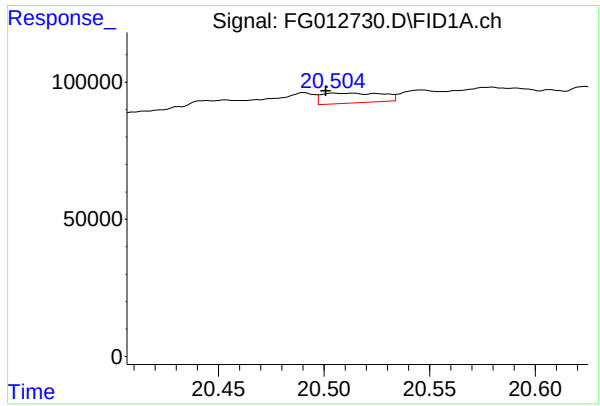

#16 N-HEXATRIACONTANE

R.T.: 20.505 min
Delta R.T.: 0.004 min
Response: 72224
Conc: 0.89 ug/ml

Instrument :

FID_G

ClientSampleId :