

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081823\
Data File : FG012722.D
Signal(s) : FID1A.ch
Acq On : 18 Aug 2023 14:57
Operator : YP\AJ
Sample : 04046-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SB-01(0-5)

Integration File: autoint1.e
Quant Time: Aug 18 23:40:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080223.M
Quant Title :
QLast Update : Wed Aug 02 18:57:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.082	1313185	11.739 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081823\
Data File : FG012722.D
Signal(s) : FID1A.ch
Acq On : 18 Aug 2023 14:57
Operator : YP\AJ
Sample : 04046-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SB-01(0-5)

Integration File: autoint1.e
Quant Time: Aug 18 23:40:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080223.M
Quant Title :
QLast Update : Wed Aug 02 18:57:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

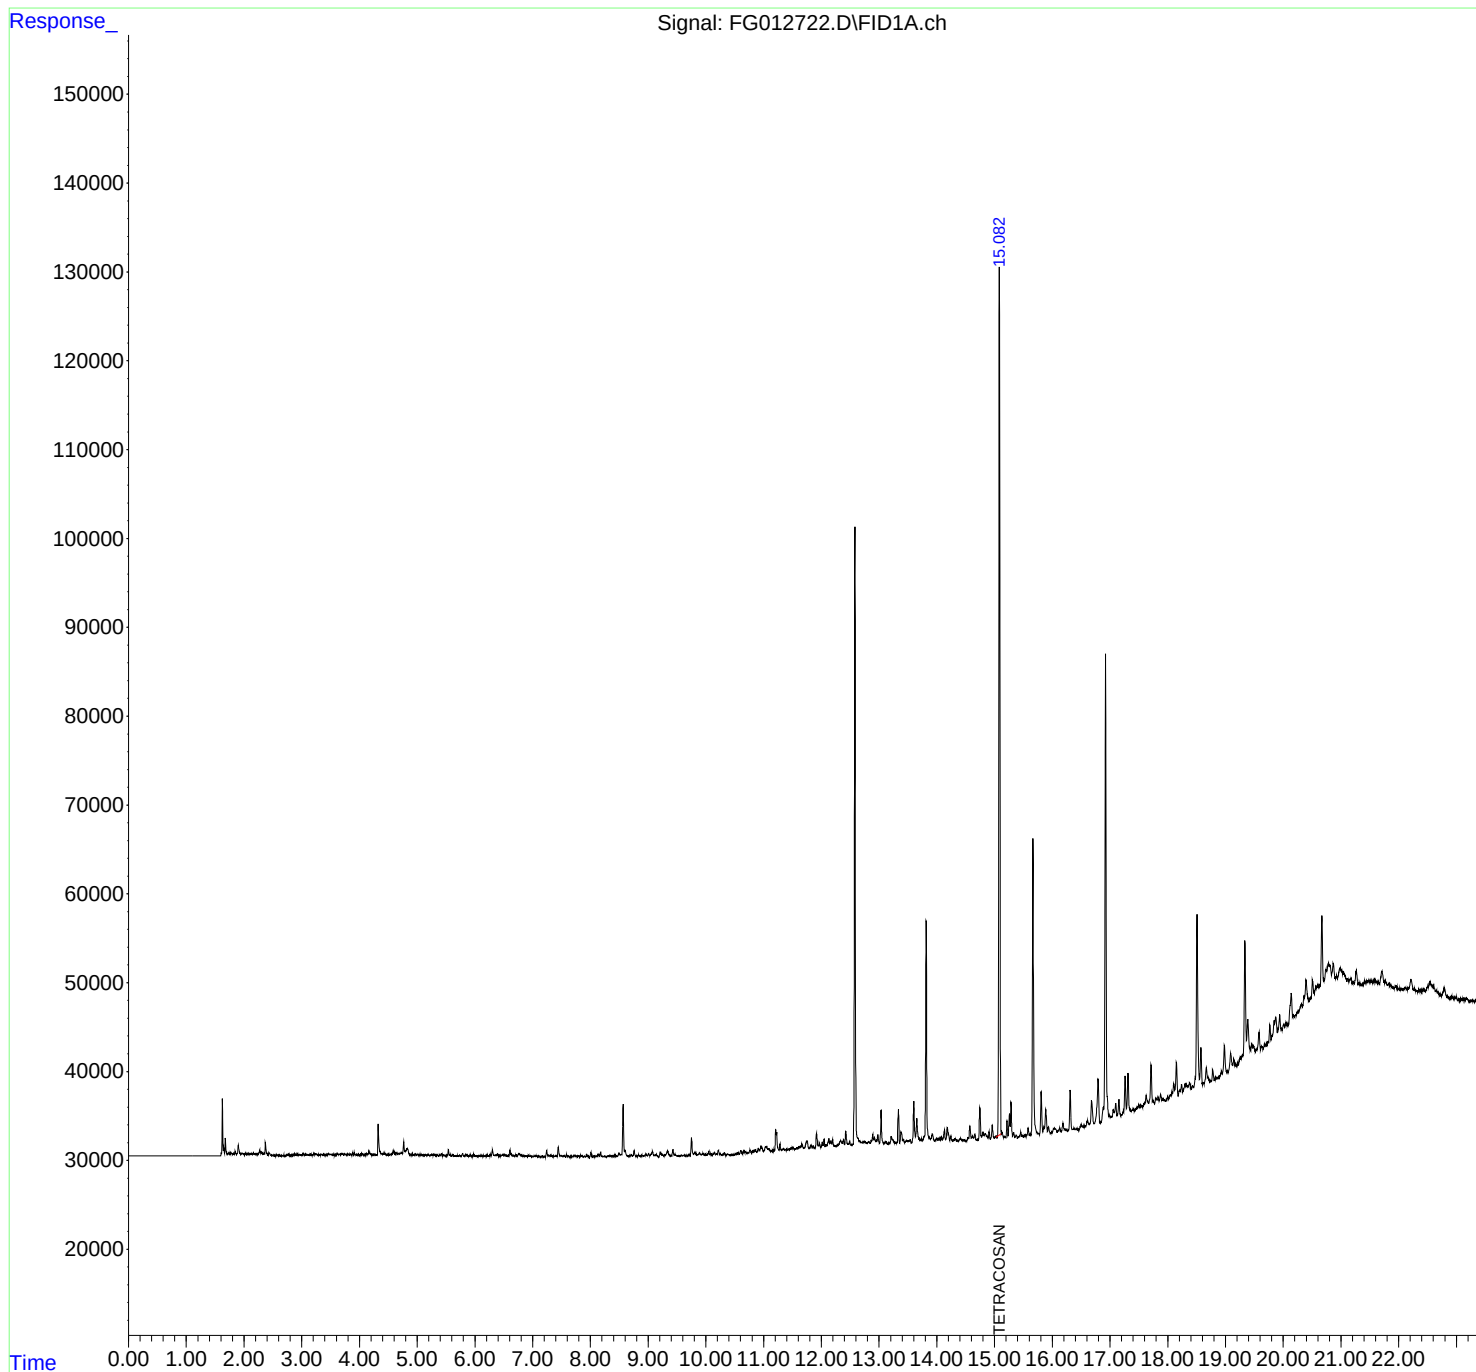

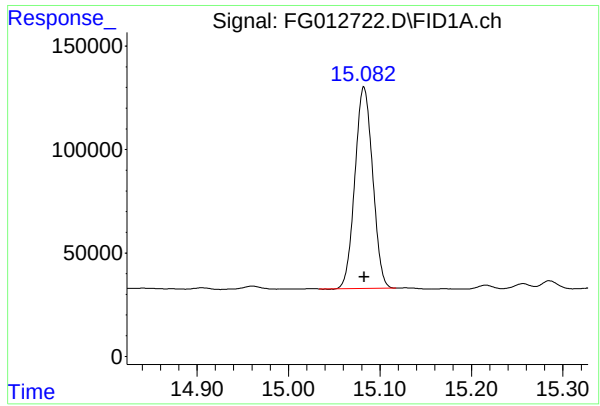

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.082 min
Delta R.T.: 0.000 min
Response: 1313185
Conc: 11.74 ug/ml

Instrument :
FID_G
ClientSampleId :
SB-01(0-5)