

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081919\
Data File : FG005644.D
Signal(s) : FID1A.ch
Acq On : 19 Aug 2019 11:39
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 20 00:45:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080819.M
Quant Title :
QLast Update : Thu Aug 08 16:03:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3)	N-DODECANE	6.477	3491620 23.834 ug/ml
12)	N-OCTACOSANE	16.927	2956063 19.554 ug/ml
13)	N-TRIACONTANE	17.814	67555 0.447 ug/ml
14)	N-DOTRIACONTANE	18.650	76431 0.571 ug/ml
15)	N-TETRATRIACONTANE	19.434	66819 0.541 ug/ml
16)	N-HEXATRIACONTANE	20.205	98161 0.851 ug/ml
18)	N-TETRACONTANE	21.891	241544 2.323 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081919\
Data File : FG005644.D
Signal(s) : FID1A.ch
Acq On : 19 Aug 2019 11:39
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 20 00:45:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080819.M
Quant Title :
QLast Update : Thu Aug 08 16:03:53 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

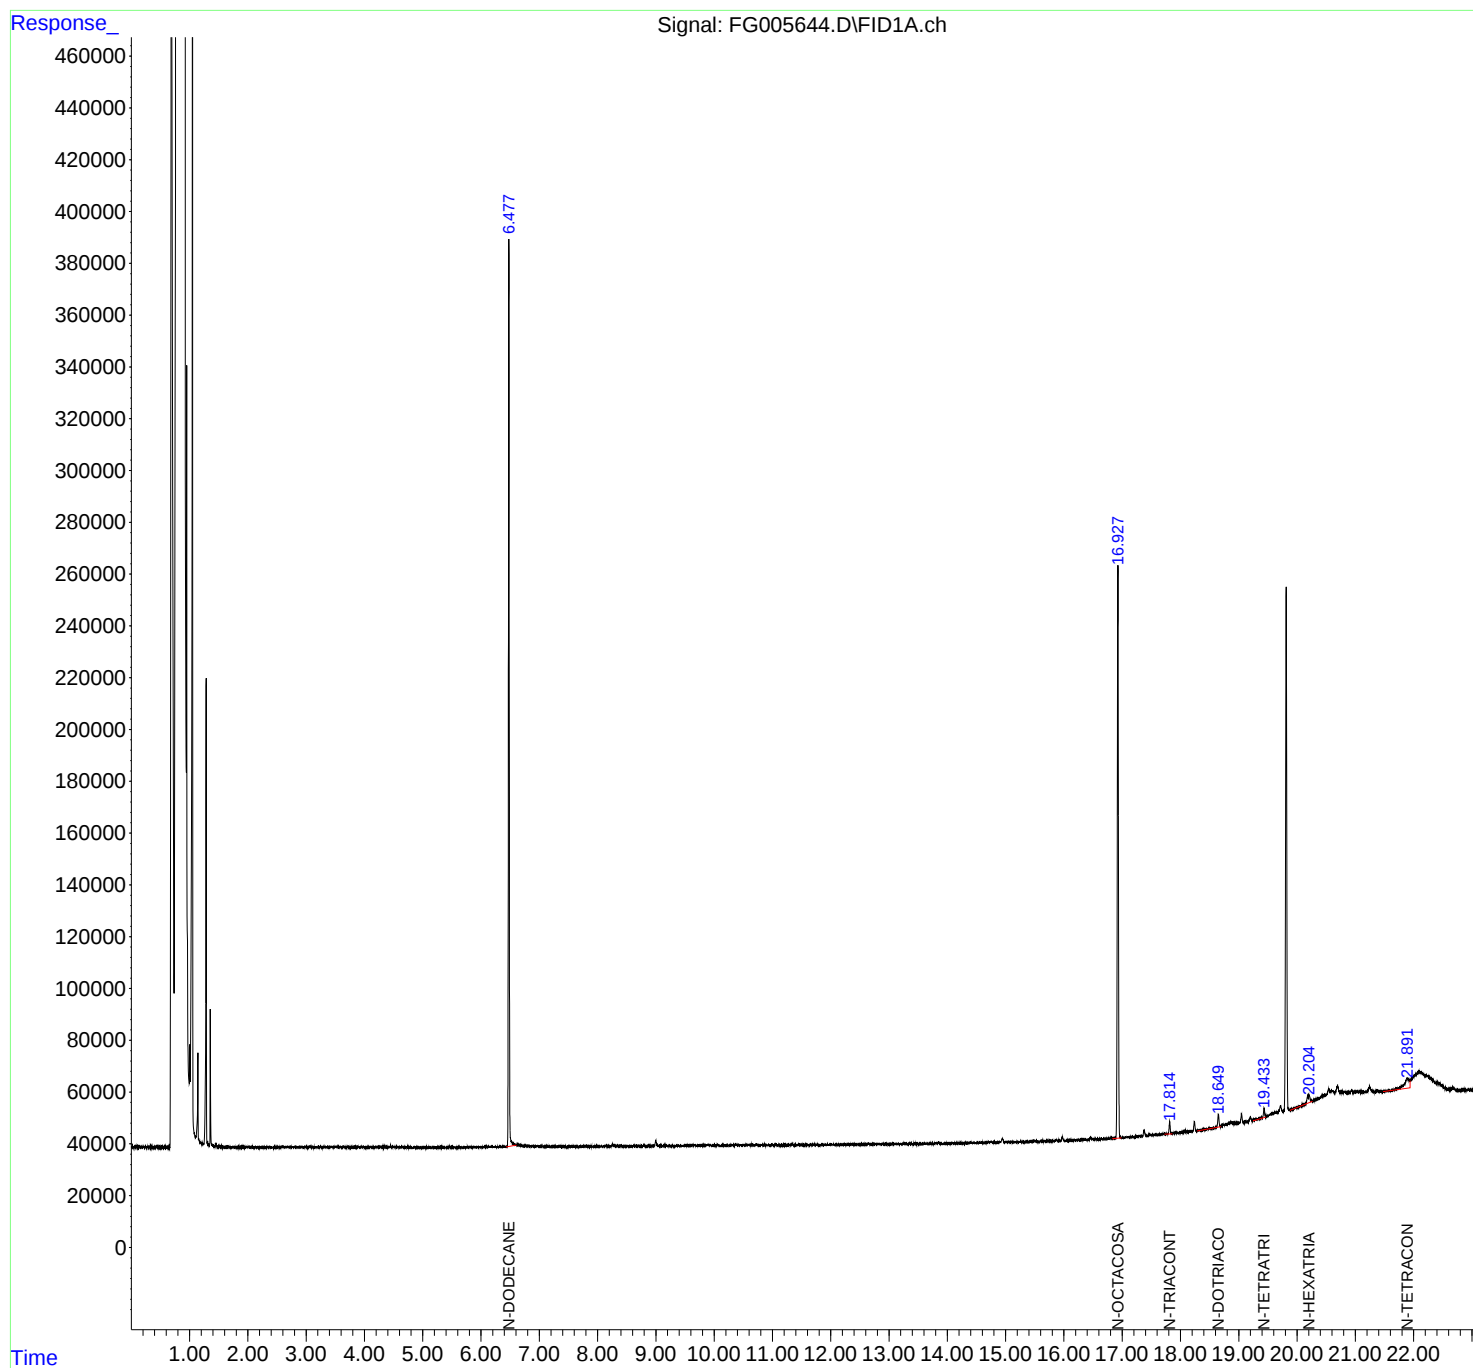

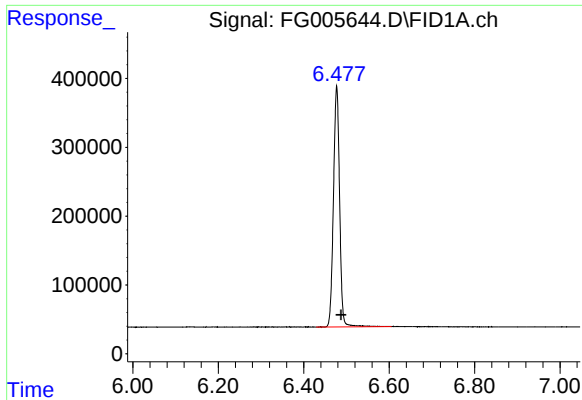


#3 N-DODECANE

R.T.: 6.477 min
Delta R.T.: -0.010 min
Response: 3491620
Conc: 23.83 ug/ml

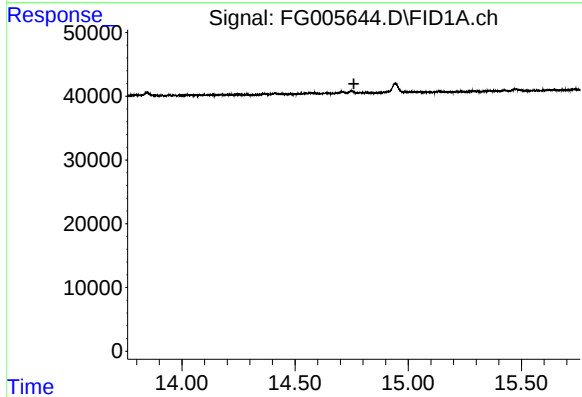


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.760 min
Response: 0
Conc: N.D.

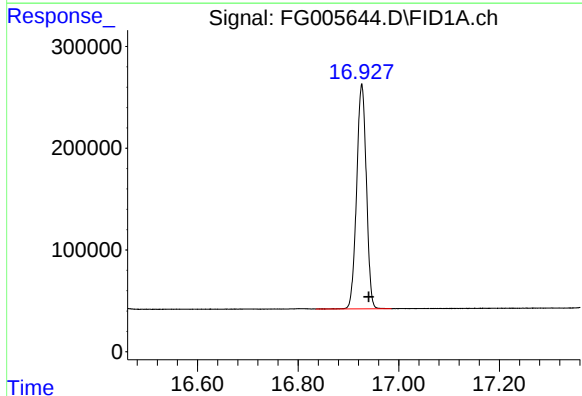


#12 N-OCTACOSANE

R.T.: 16.927 min
Delta R.T.: -0.013 min
Response: 2956063
Conc: 19.55 ug/ml

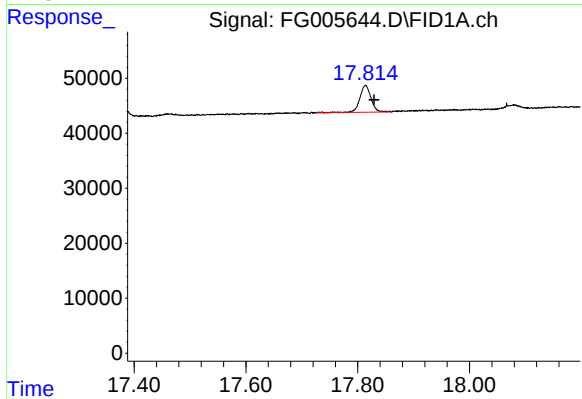


#13 N-TRIACONTANE

R.T.: 17.814 min
Delta R.T.: -0.015 min
Response: 67555
Conc: 0.45 ug/ml

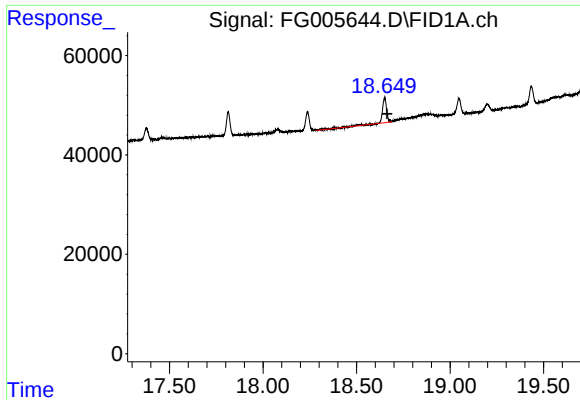


#14 N-DOTRIACONTANE

R.T.: 18.650 min
Delta R.T.: -0.014 min
Response: 76431
Conc: 0.57 ug/ml

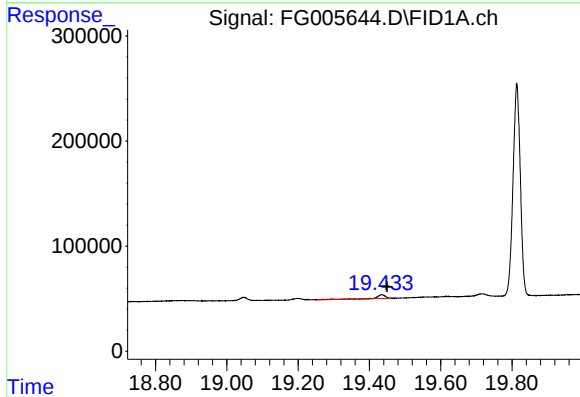


#15 N-TETRATRIACONTANE

R.T.: 19.434 min
Delta R.T.: -0.015 min
Response: 66819
Conc: 0.54 ug/ml

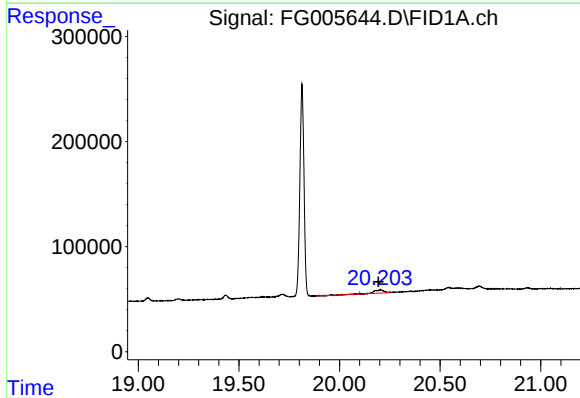

#16 N-HEXATRIACONTANE

R.T.: 20.205 min
Delta R.T.: 0.012 min
Response: 98161
Conc: 0.85 ug/ml

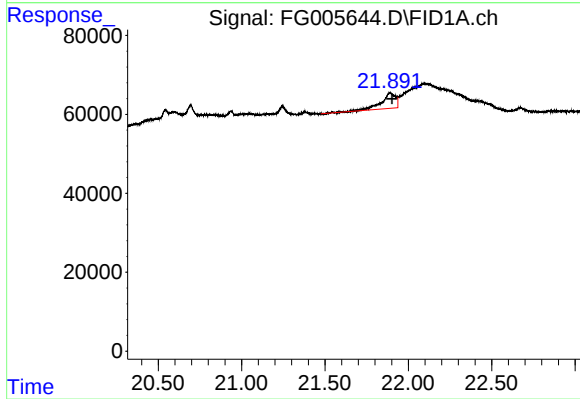

#18 N-TETRACONTANE

R.T.: 21.891 min
Delta R.T.: -0.011 min
Response: 241544
Conc: 2.32 ug/ml