

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081922\
Data File : FG010386.D
Signal(s) : FID1A.ch
Acq On : 19 Aug 2022 13:41
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 19 18:44:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG072822.M
Quant Title :
QLast Update : Thu Jul 28 15:10:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.500	2497302	18.169 ug/ml
12)	N-OCTACOSANE	16.968	2295289	16.623 ug/ml
15)	N-TETRATRIACONTANE	19.473	43693	0.349 ug/ml
17)	N-OCTATRIACONTANE	20.922	101135	0.890 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081922\
Data File : FG010386.D
Signal(s) : FID1A.ch
Acq On : 19 Aug 2022 13:41
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 19 18:44:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG072822.M
Quant Title :
QLast Update : Thu Jul 28 15:10:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

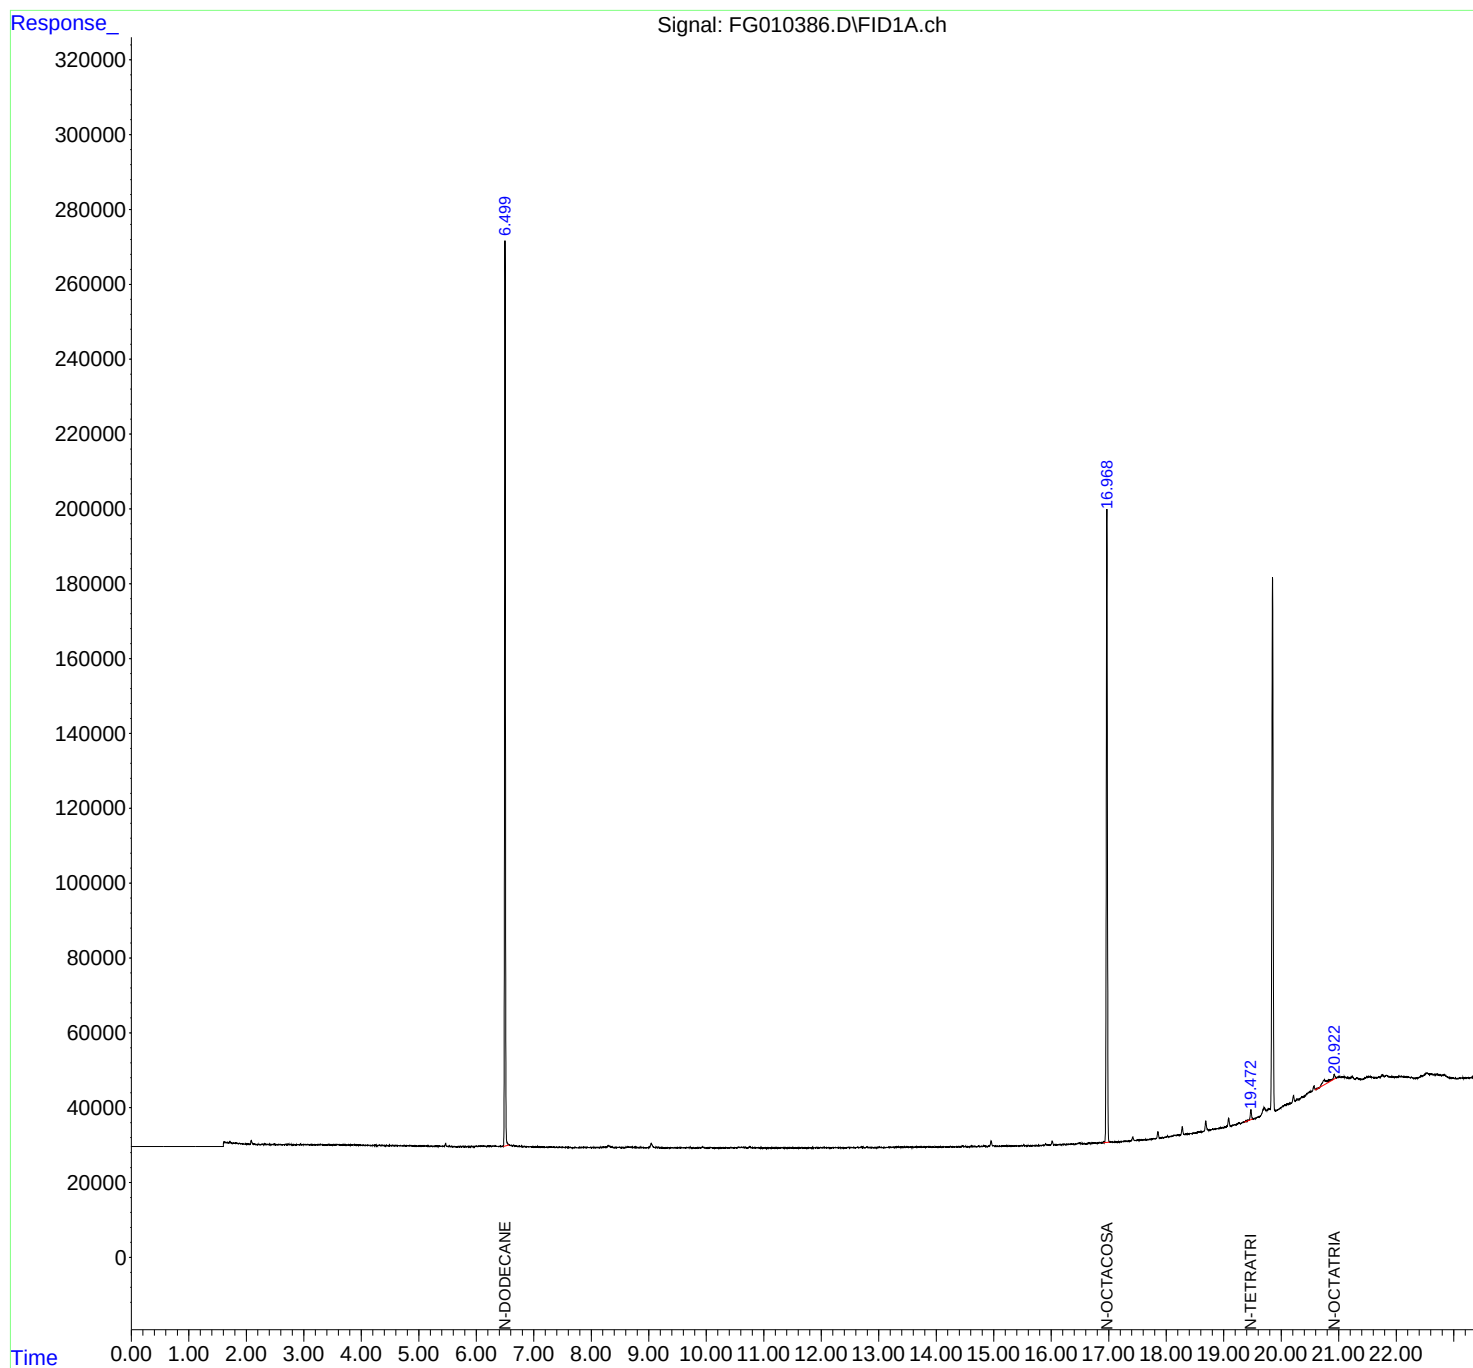


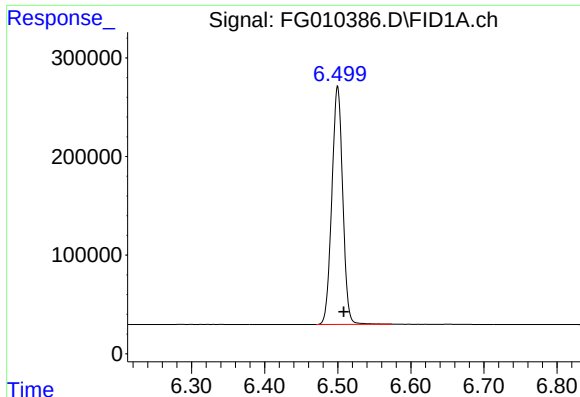

#3 N-DODECANE


R.T.: 6.500 min
Delta R.T.: -0.008 min
Response: 2497302
Conc: 18.17 ug/ml

Instrument :
FID_G
ClientSampleId :

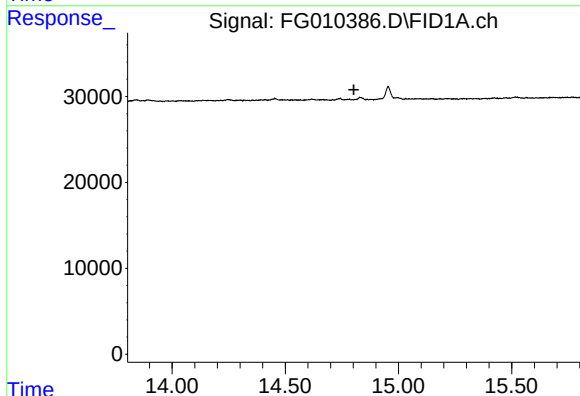


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.803 min
Response: 0
Conc: N.D.

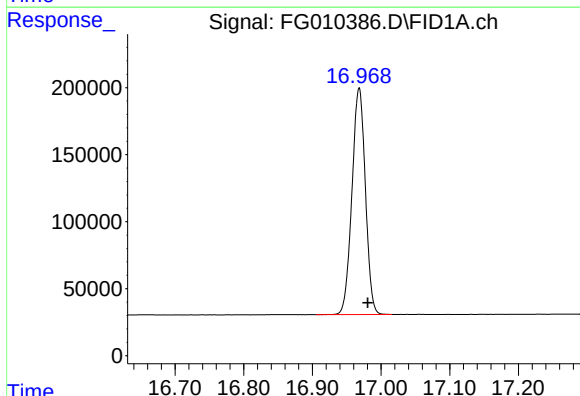


#12 N-OCTACOSANE

R.T.: 16.968 min
Delta R.T.: -0.012 min
Response: 2295289
Conc: 16.62 ug/ml

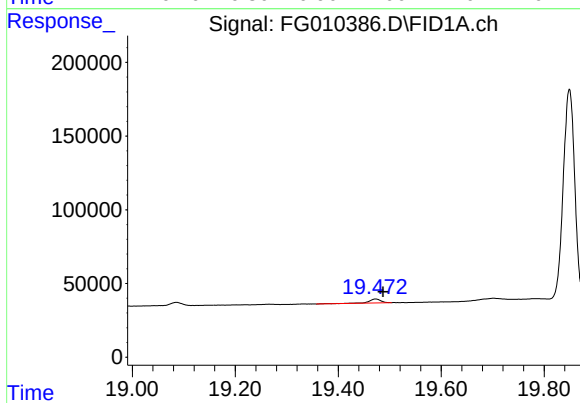

#15 N-TETRATRIACONTANE

R.T.: 19.473 min
Delta R.T.: -0.015 min
Response: 43693
Conc: 0.35 ug/ml

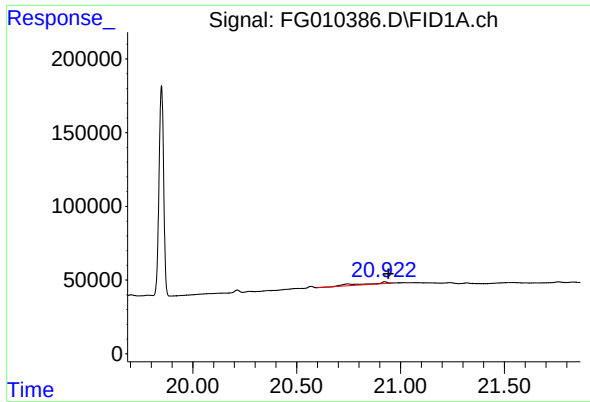

#17 N-OCTATRIACONTANE

R.T.: 20.922 min
Delta R.T.: -0.020 min
Response: 101135
Conc: 0.89 ug/ml

Instrument :

FID_G

ClientSampleId :