

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081922\
 Data File : FG010390.D
 Signal(s) : FID1A.ch
 Acq On : 19 Aug 2022 17:31
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 19 18:44:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG072822.M
 Quant Title :
 QLast Update : Thu Jul 28 15:10:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.791	1997253	15.722 ug/ml
Target Compounds			
16) N-HEXATRIACONTANE	20.211	32303	0.280 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG081922\
Data File : FG010390.D
Signal(s) : FID1A.ch
Acq On : 19 Aug 2022 17:31
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 19 18:44:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG072822.M
Quant Title :
QLast Update : Thu Jul 28 15:10:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

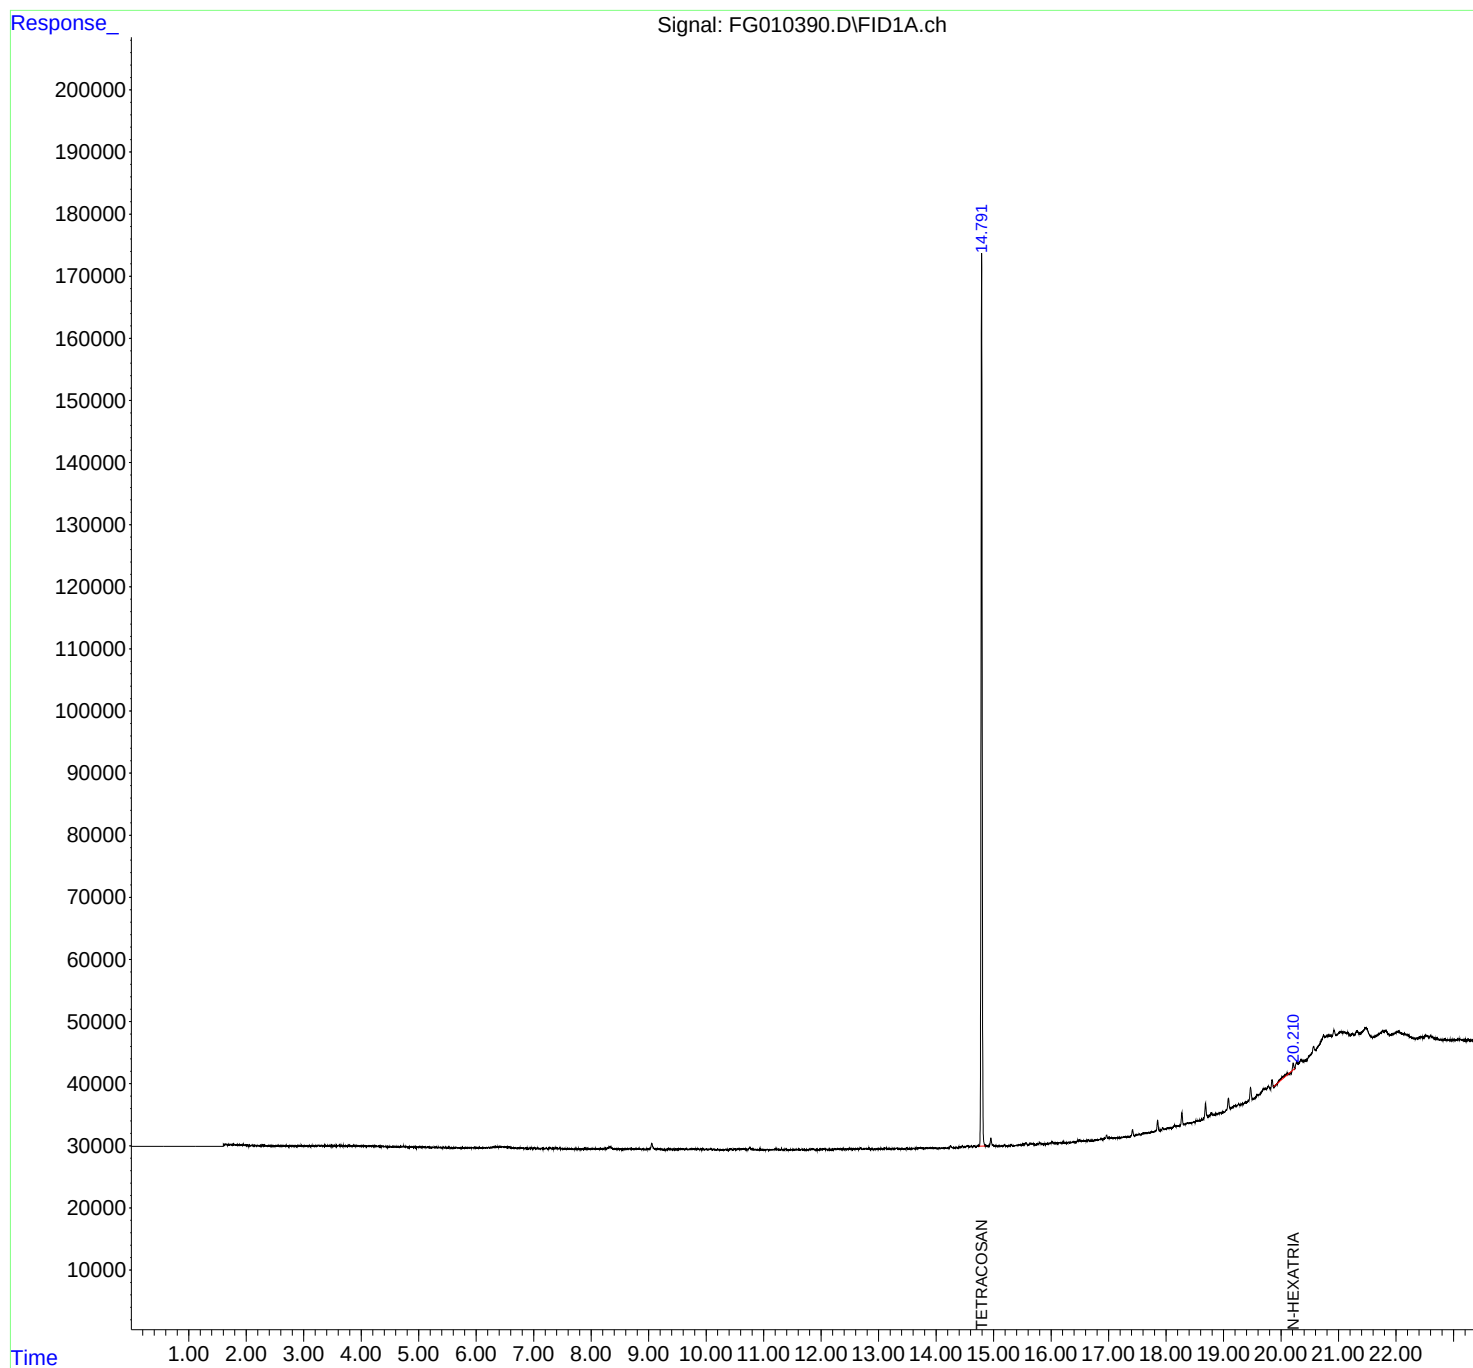


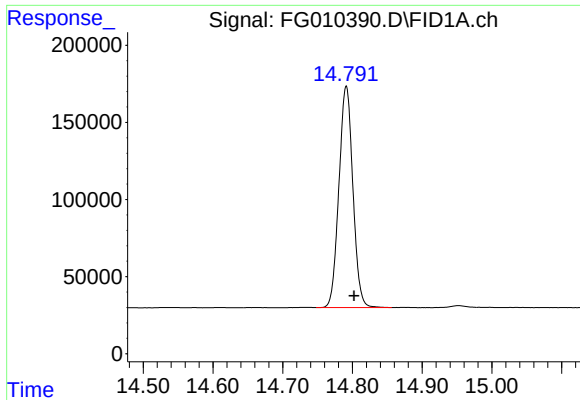

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.791 min
Delta R.T.: -0.011 min
Response: 1997253
Conc: 15.72 ug/ml

Instrument :
FID_G
ClientSampleId :

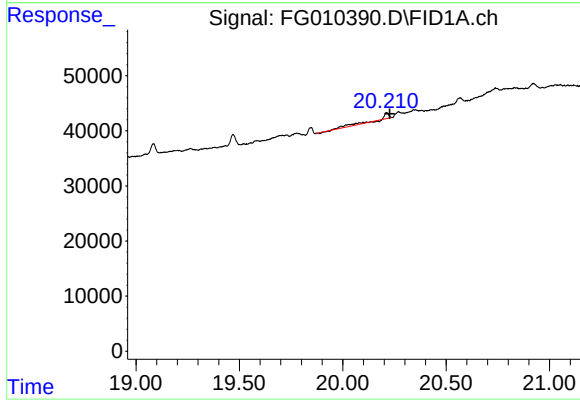

#16 N-HEXATRIACONTANE

R.T.: 20.211 min
Delta R.T.: -0.017 min
Response: 32303
Conc: 0.28 ug/ml