

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG082019\
Data File : FG005649.D
Signal(s) : FID1A.ch
Acq On : 20 Aug 2019 10:03
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 20 22:39:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080819.M
Quant Title :
QLast Update : Thu Aug 08 16:03:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
10)	N-TETRACOSANE	14.939	55968	0.385 ug/ml
14)	N-DOTRIACONTANE	18.654	46052	0.344 ug/ml
15)	N-TETRATRIACONTANE	19.440	10000	0.081 ug/ml
16)	N-HEXATRIACONTANE	20.211	79288	0.688 ug/ml
18)	N-TETRACONTANE	21.897	44369	0.427 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG082019\
Data File : FG005649.D
Signal(s) : FID1A.ch
Acq On : 20 Aug 2019 10:03
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 20 22:39:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080819.M
Quant Title :
QLast Update : Thu Aug 08 16:03:53 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

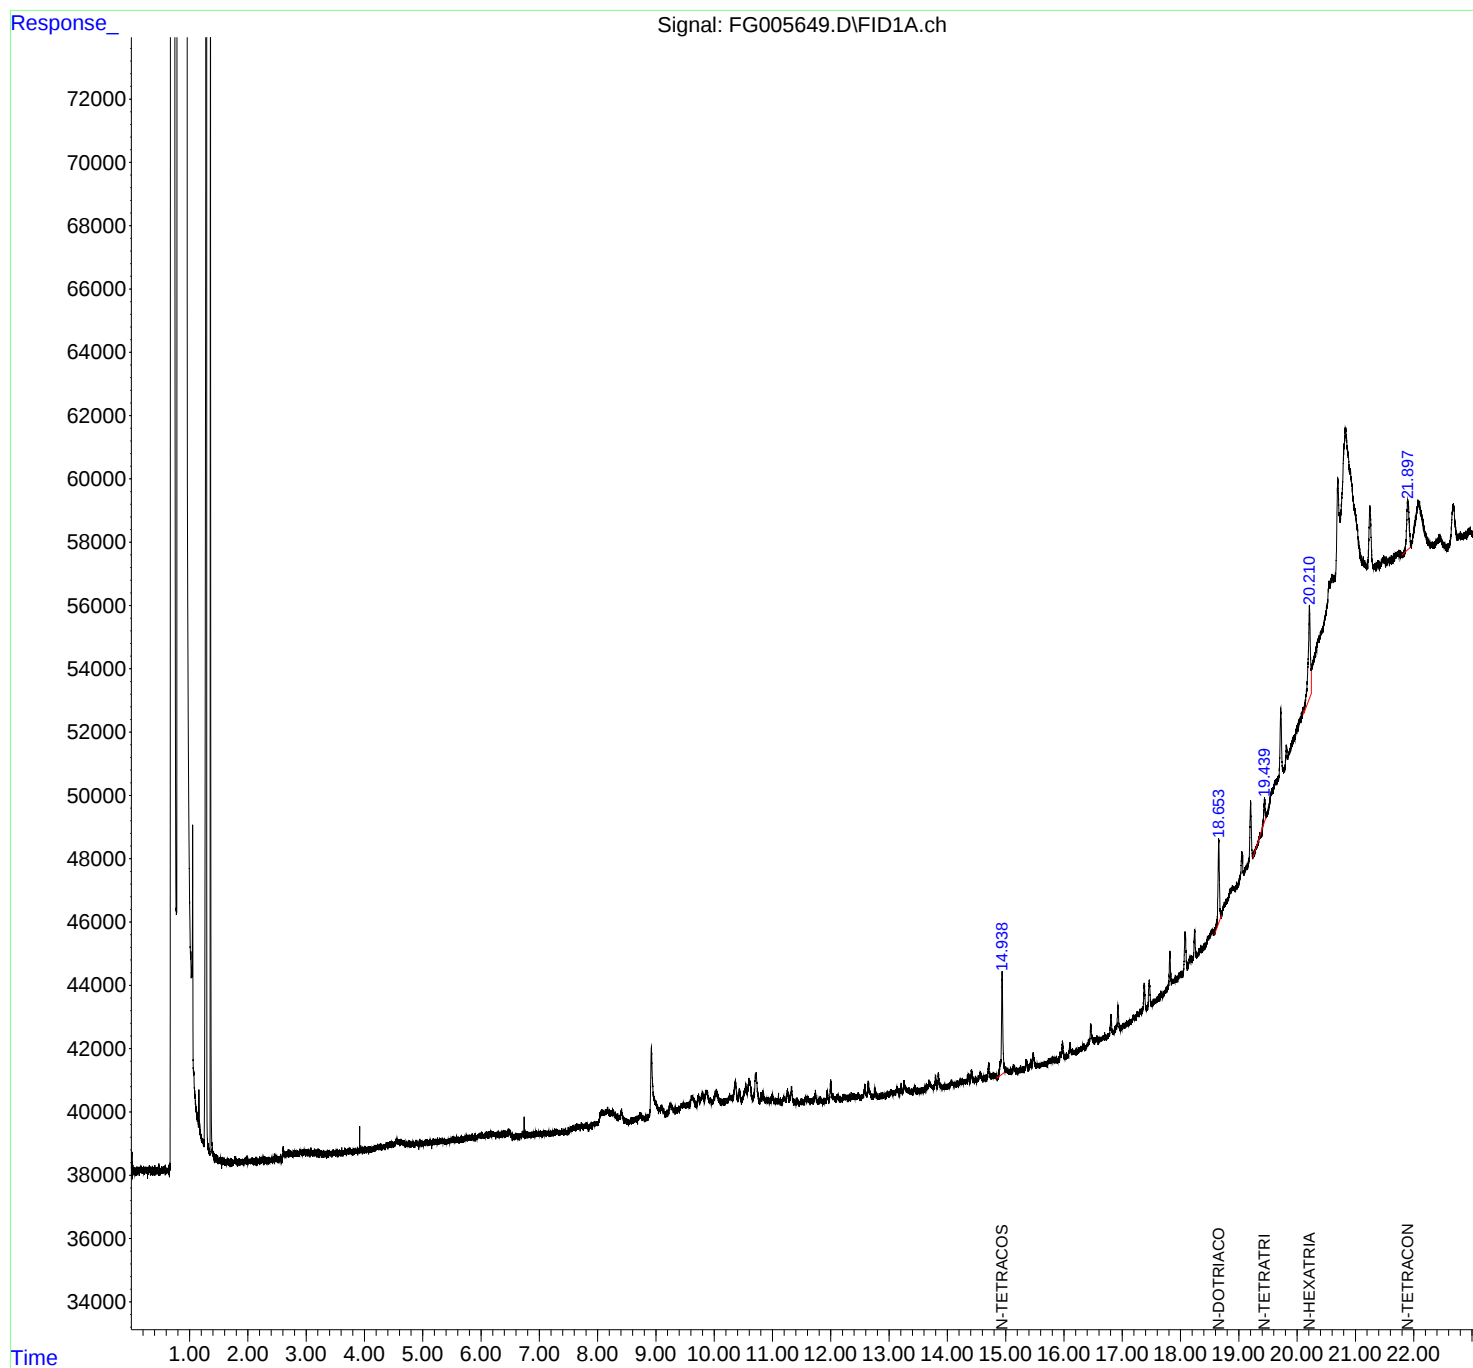

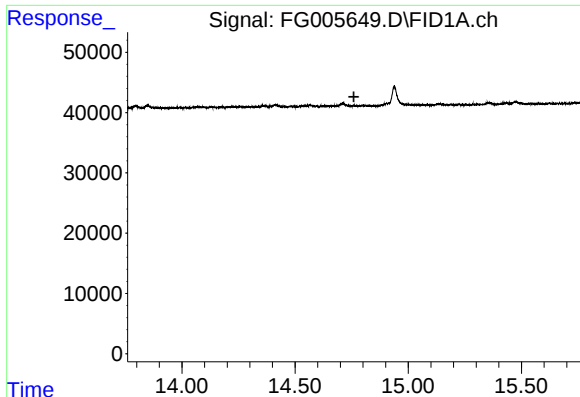


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.760 min
Response: 0
Conc: N.D.

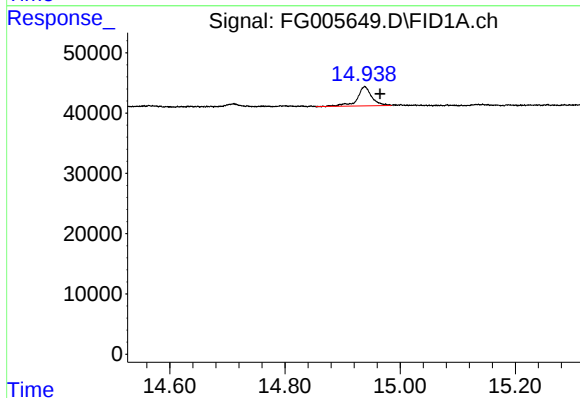


#10 N-TETRACOSANE

R.T.: 14.939 min
Delta R.T.: -0.026 min
Response: 55968
Conc: 0.39 ug/ml

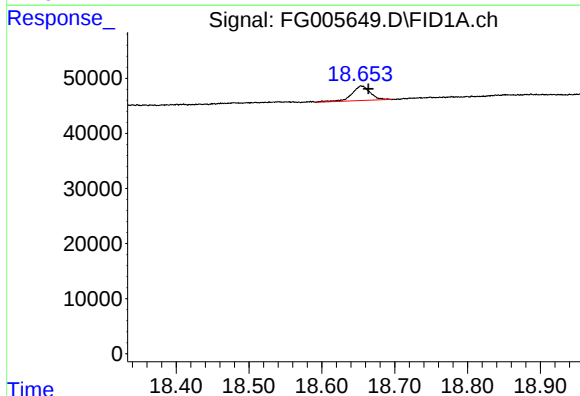


#14 N-DOTRIACONTANE

R.T.: 18.654 min
Delta R.T.: -0.010 min
Response: 46052
Conc: 0.34 ug/ml

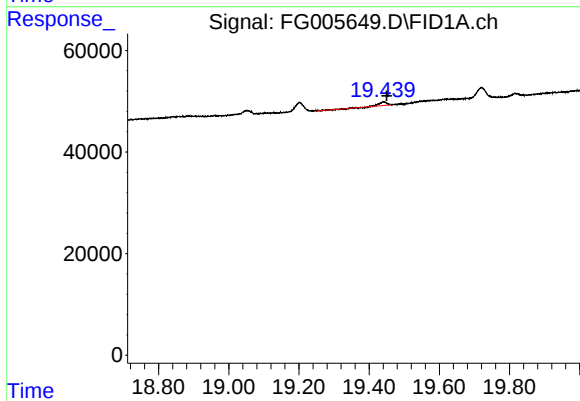


#15 N-TETRATRIACONTANE

R.T.: 19.440 min
Delta R.T.: -0.010 min
Response: 10000
Conc: 0.08 ug/ml

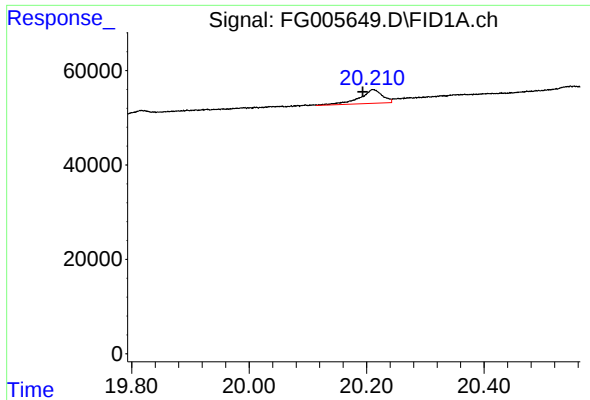

#16 N-HEXATRIACONTANE

R.T.: 20.211 min
Delta R.T.: 0.017 min
Response: 79288
Conc: 0.69 ug/ml

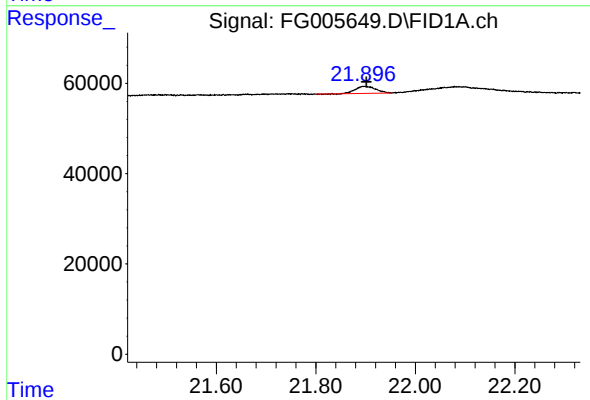

#18 N-TETRACONTANE

R.T.: 21.897 min
Delta R.T.: -0.005 min
Response: 44369
Conc: 0.43 ug/ml