

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG082024\  
Data File : FG014123.D  
Signal(s) : FID1A.ch  
Acq On : 20 Aug 2024 14:26  
Operator : YP\AJ  
Sample : P3670-01  
Misc :  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Aug 21 02:53:51 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG081624.M  
Quant Title :  
QLast Update : Fri Aug 16 10:59:42 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.932 | 1160984  | 10.986 ug/ml |
| Target Compounds              |        |          |              |
| 7) N-EICOSANE                 | 12.874 | 93905    | 0.789 ug/ml  |
| 12) N-OCTACOSANE              | 17.157 | 84913    | 0.720 ug/ml  |
| 14) N-DOTRIACONTANE           | 18.827 | 173321   | 1.450 ug/ml  |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG082024\  
Data File : FG014123.D  
Signal(s) : FID1A.ch  
Acq On : 20 Aug 2024 14:26  
Operator : YP\AJ  
Sample : P3670-01  
Misc :  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Aug 21 02:53:51 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG081624.M  
Quant Title :  
QLast Update : Fri Aug 16 10:59:42 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

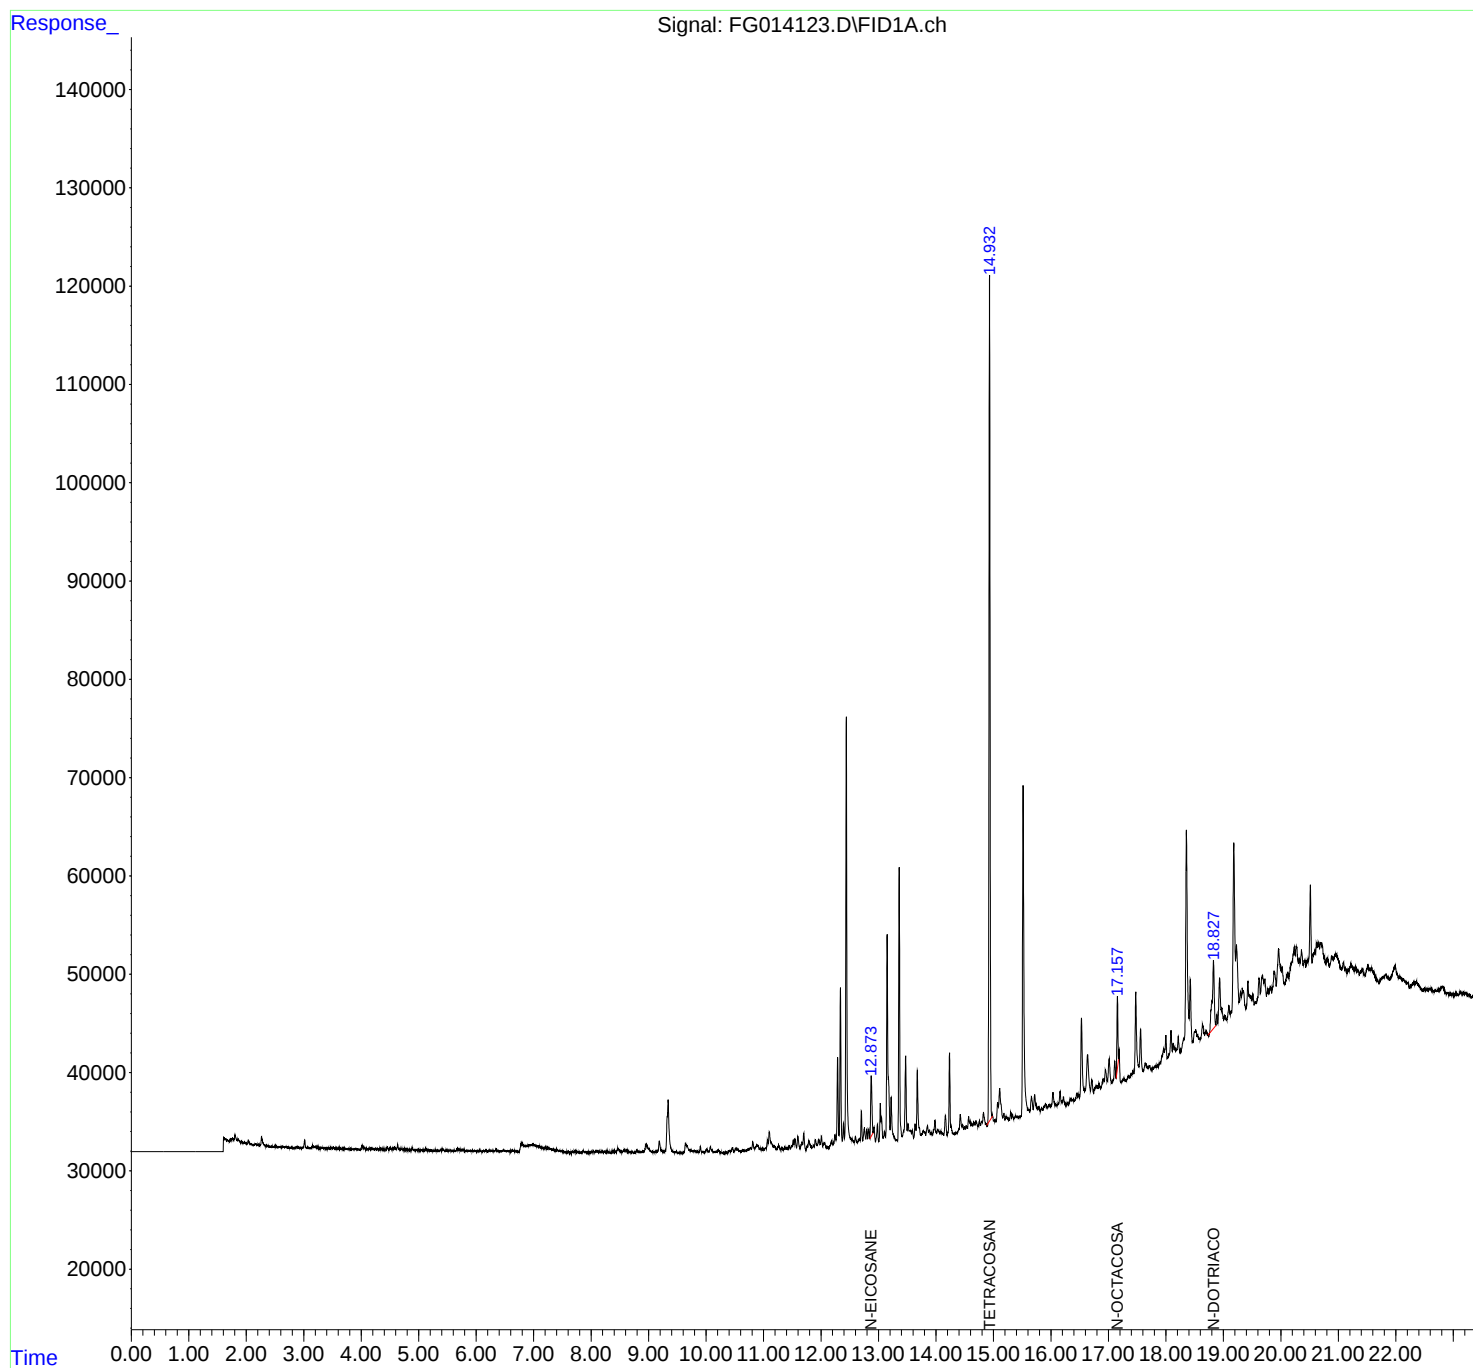


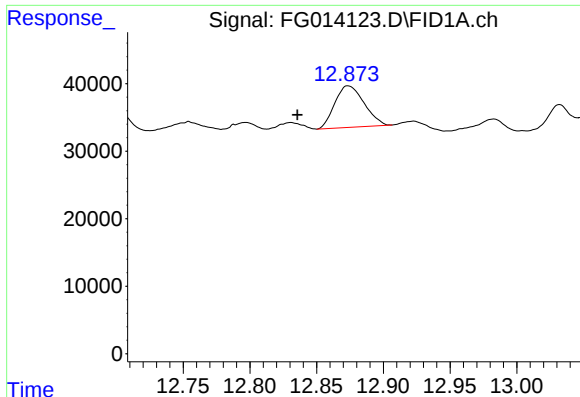

#7 N-EICOSANE


R.T.: 12.874 min  
Delta R.T.: 0.038 min  
Response: 93905  
Conc: 0.79 ug/ml

Instrument :  
FID\_G  
ClientSampleId :

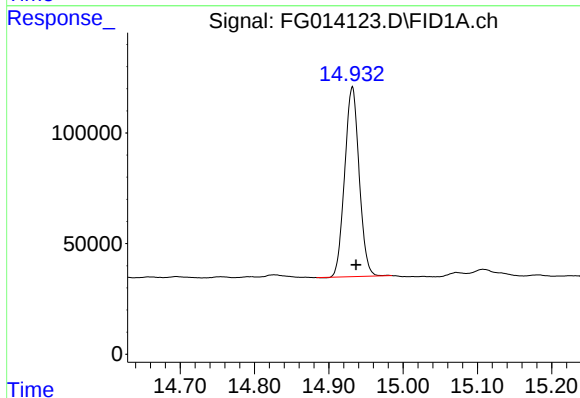


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.932 min  
Delta R.T.: -0.005 min  
Response: 1160984  
Conc: 10.99 ug/ml

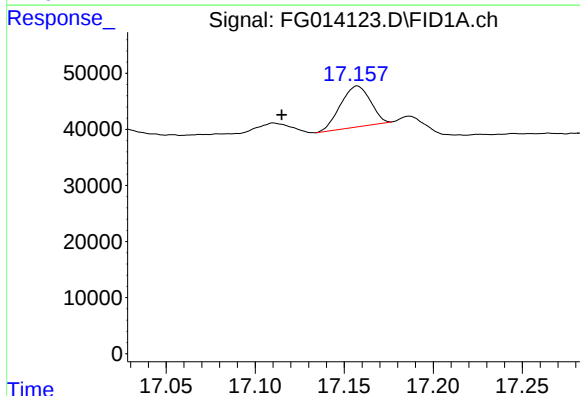

#12 N-OCTACOSANE

R.T.: 17.157 min  
Delta R.T.: 0.043 min  
Response: 84913  
Conc: 0.72 ug/ml

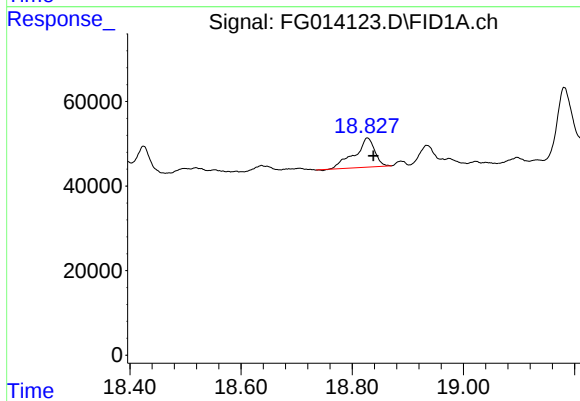

#14 N-DOTRIACONTANE

R.T.: 18.827 min  
Delta R.T.: -0.011 min  
Response: 173321  
Conc: 1.45 ug/ml