

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG082118\
Data File : FG002140.D
Signal(s) : FID1A.ch
Acq On : 21 Aug 2018 11:40
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 22 01:56:53 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG073018.M
Quant Title :
QLast Update : Mon Jul 30 13:56:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.219	3812813	25.380 ug/ml
12) N-OCTACOSANE	16.628	3646634	26.138 ug/ml
13) N-TRIACONTANE	17.514	171007	1.252 ug/ml
14) N-DOTRIACONTANE	18.348	178487	1.441 ug/ml
15) N-TETRATRIACONTANE	19.134	116947	1.076 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG082118\
Data File : FG002140.D
Signal(s) : FID1A.ch
Acq On : 21 Aug 2018 11:40
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 22 01:56:53 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG073018.M
Quant Title :
QLast Update : Mon Jul 30 13:56:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

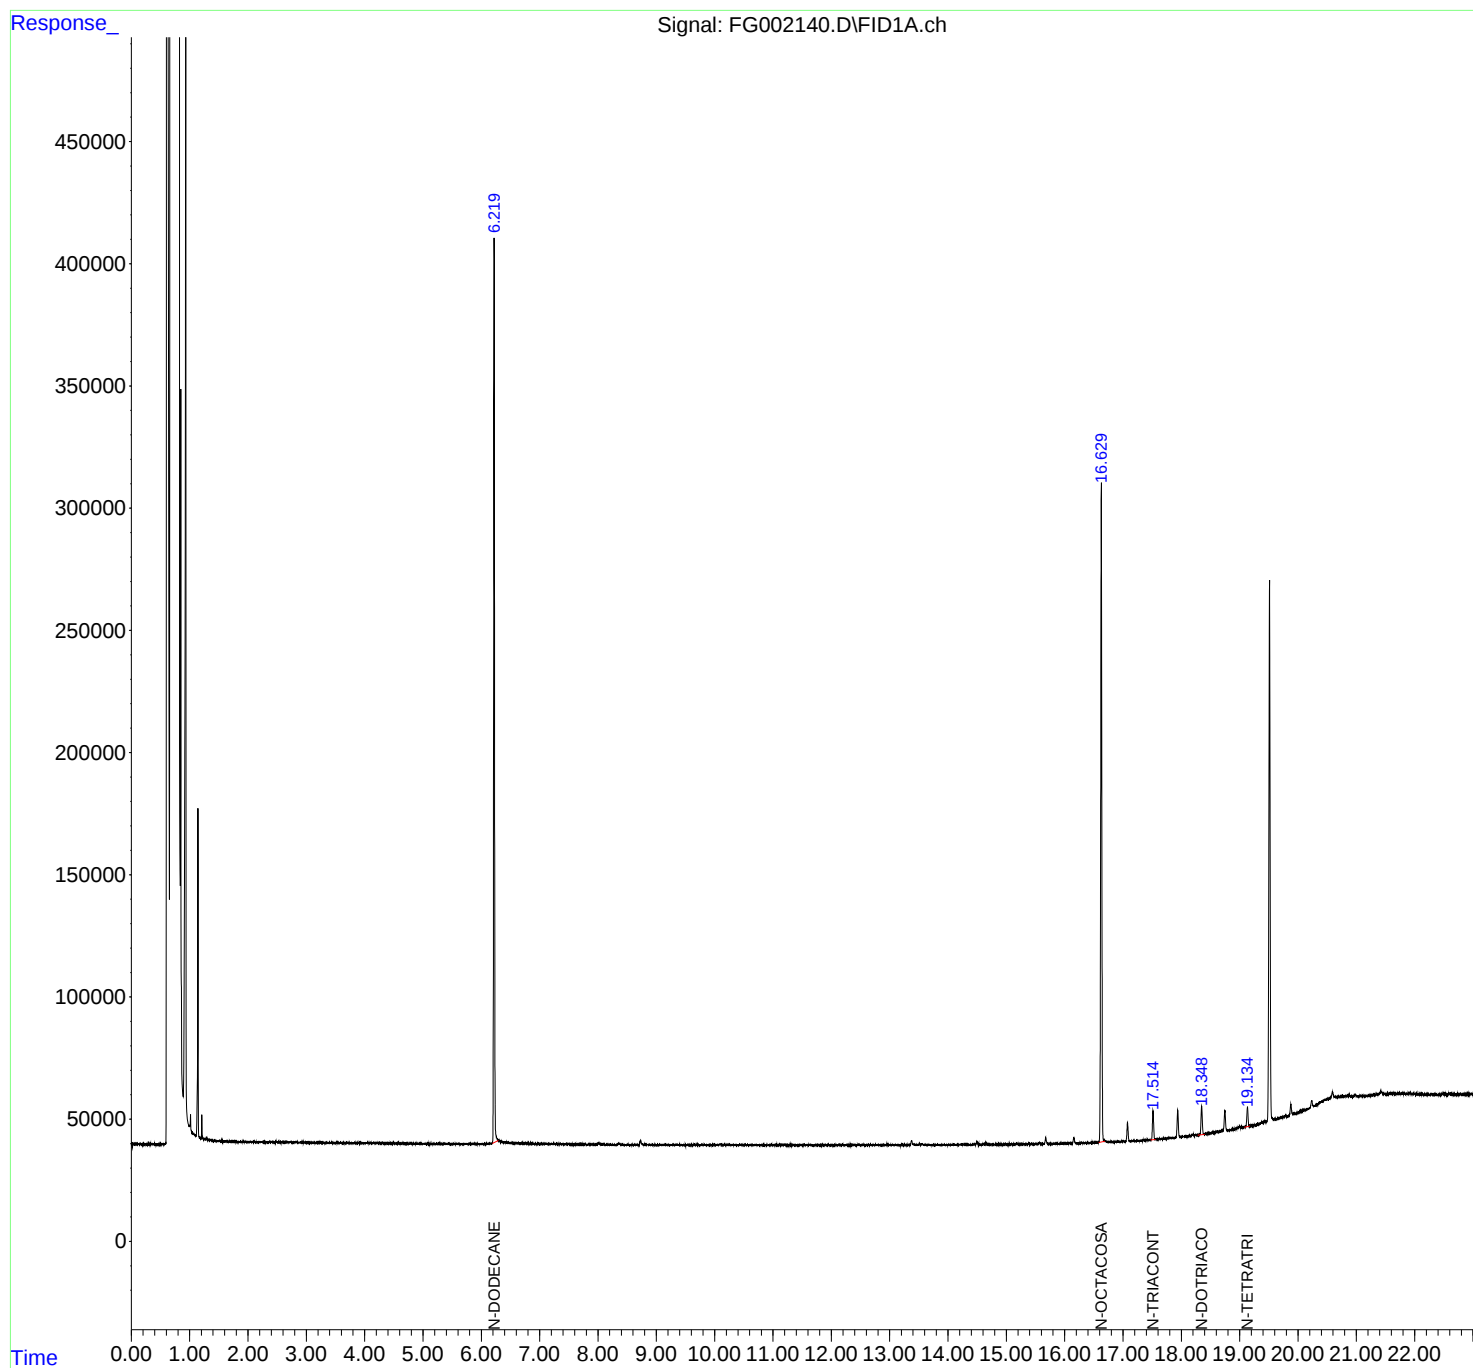


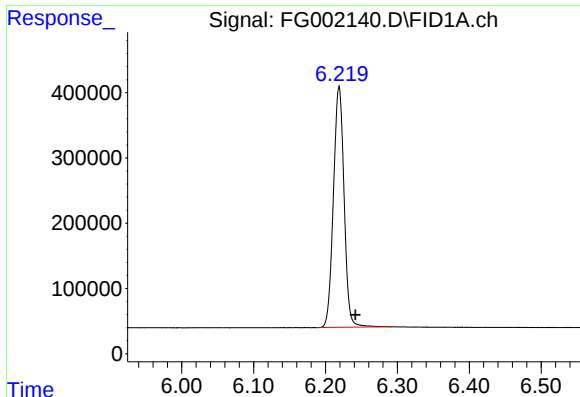

#3 N-DODECANE


R.T.: 6.219 min
Delta R.T.: -0.023 min
Response: 3812813
Conc: 25.38 ug/ml

Instrument :
FID_G
ClientSampleId :

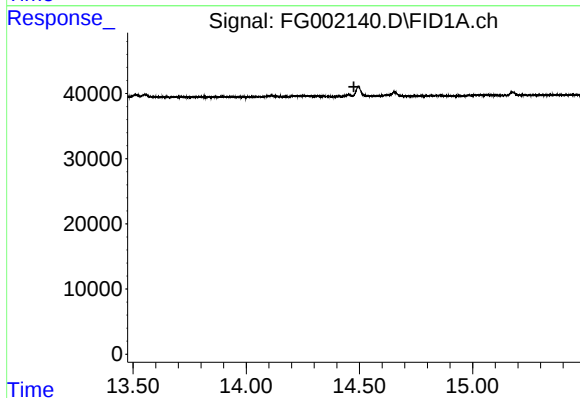


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.475 min
Response: 0
Conc: N.D.

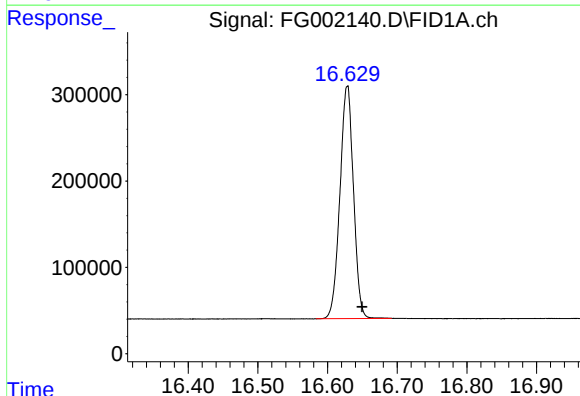


#12 N-OCTACOSANE

R.T.: 16.628 min
Delta R.T.: -0.021 min
Response: 3646634
Conc: 26.14 ug/ml

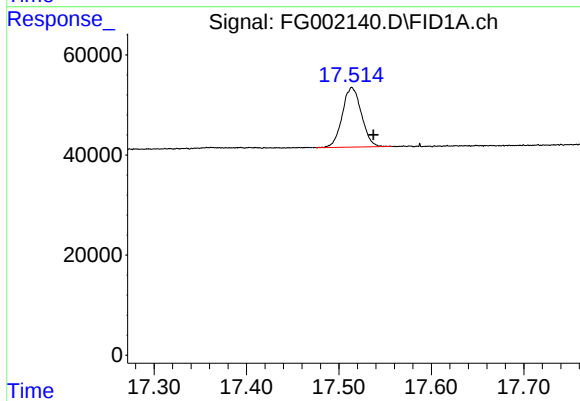

#13 N-TRIACONTANE


R.T.: 17.514 min
Delta R.T.: -0.023 min
Response: 171007
Conc: 1.25 ug/ml

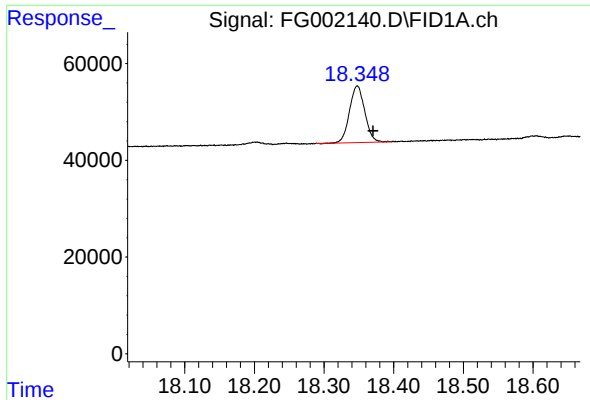

#14 N-DOTRIACONTANE

R.T.: 18.348 min
Delta R.T.: -0.022 min
Response: 178487
Conc: 1.44 ug/ml

Instrument :
FID_G
ClientSampleId :

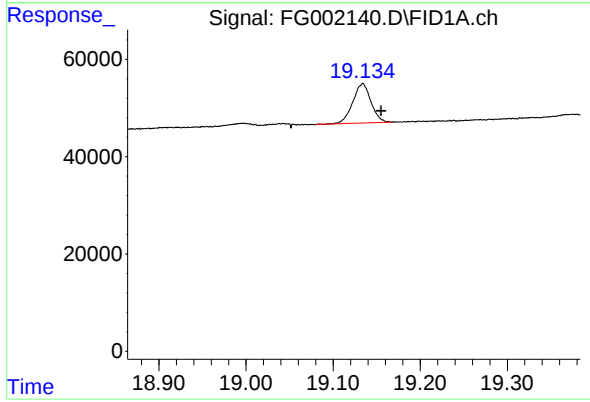

#15 N-TETRATRIACONTANE

R.T.: 19.134 min
Delta R.T.: -0.021 min
Response: 116947
Conc: 1.08 ug/ml