

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG082118\
Data File : FG002150.D
Signal(s) : FID1A.ch
Acq On : 21 Aug 2018 18:24
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 22 01:58:46 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG073018.M
Quant Title :
QLast Update : Mon Jul 30 13:56:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.455	2305984	18.294 ug/ml
Target Compounds				
16)	N-HEXATRIACONTANE	19.891	38898	0.405 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG082118\
Data File : FG002150.D
Signal(s) : FID1A.ch
Acq On : 21 Aug 2018 18:24
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampled :

Integration File: autoint1.e
Quant Time: Aug 22 01:58:46 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG073018.M
Quant Title :
QLast Update : Mon Jul 30 13:56:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

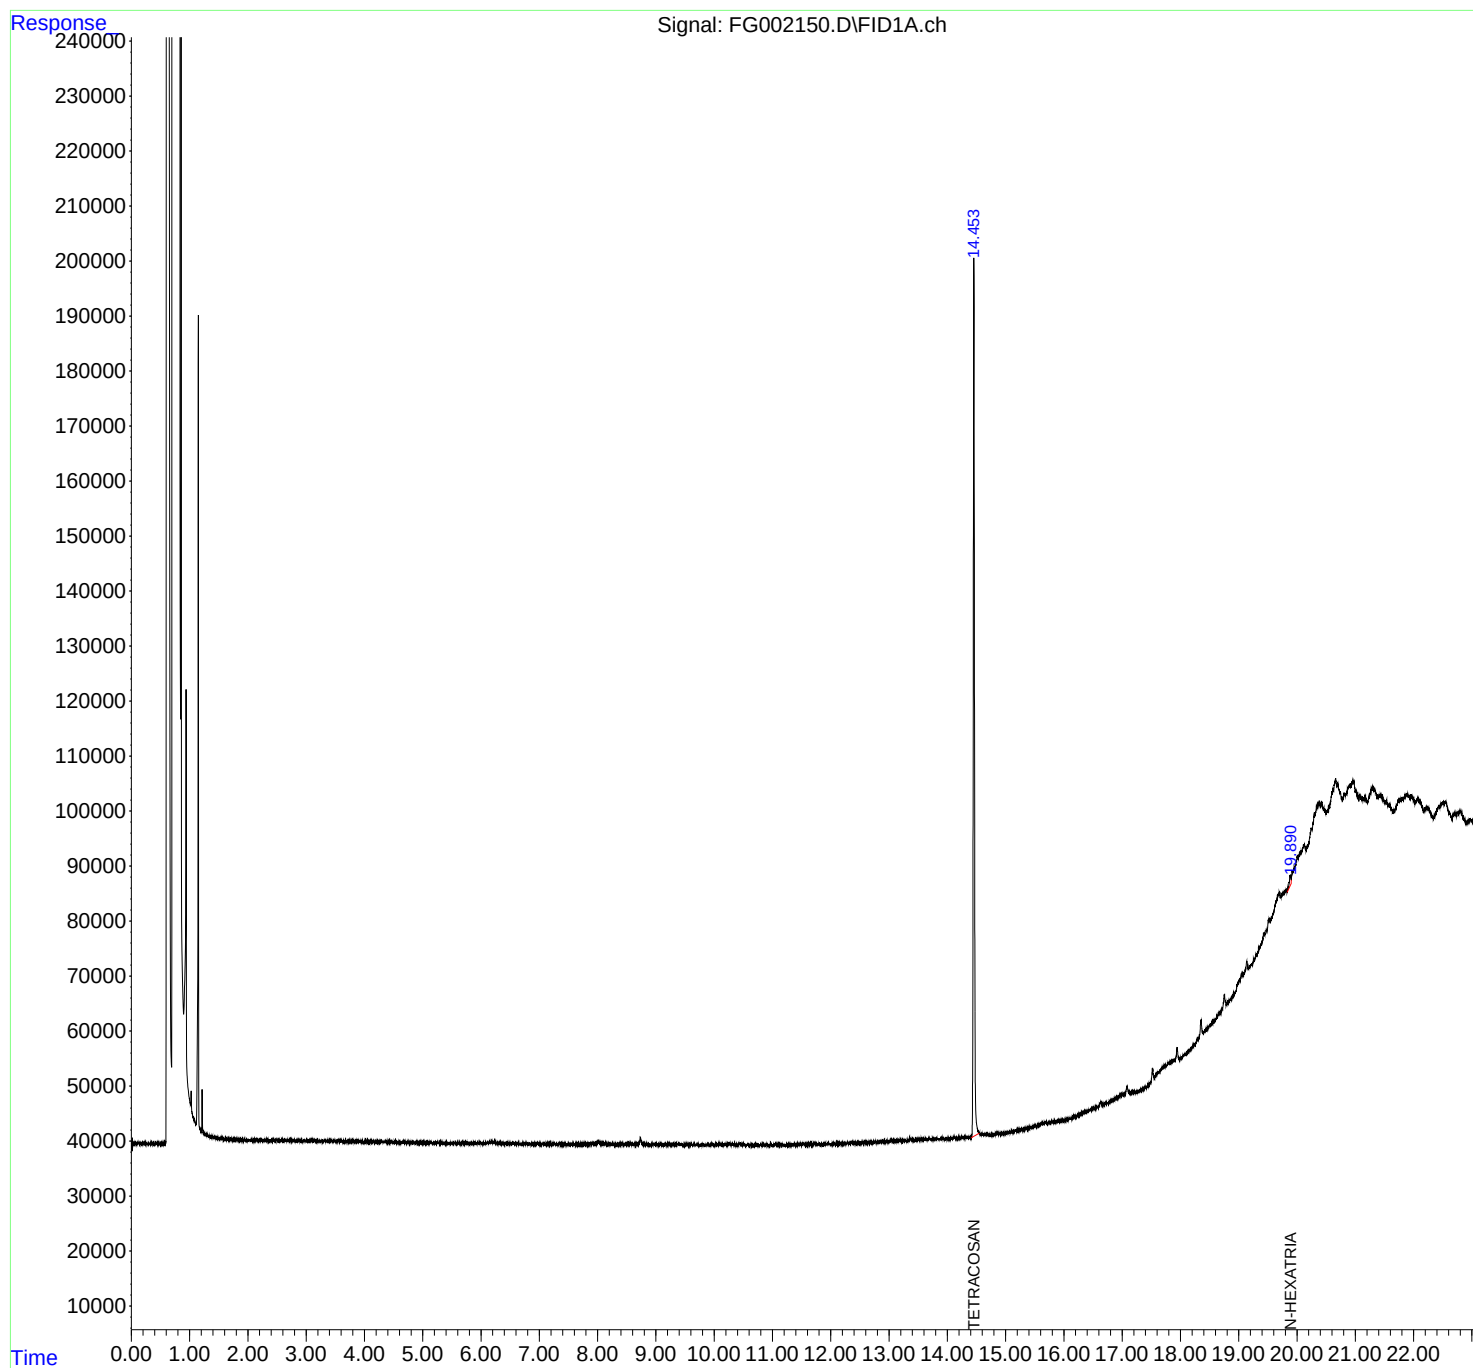


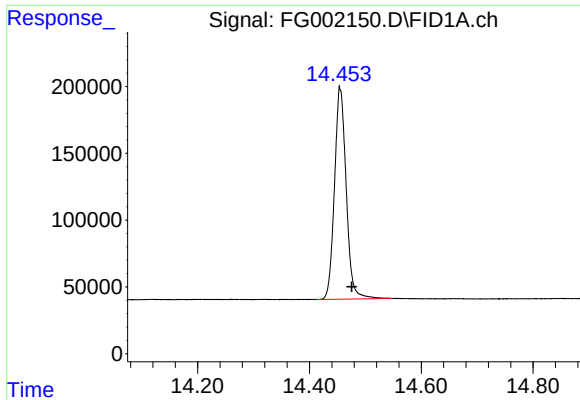

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.455 min
Delta R.T.: -0.021 min
Response: 2305984
Conc: 18.29 ug/ml

Instrument :
FID_G
ClientSampleId :

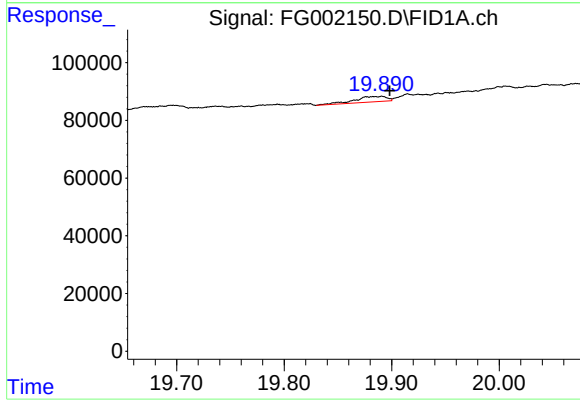

#16 N-HEXATRIACONTANE

R.T.: 19.891 min
Delta R.T.: -0.008 min
Response: 38898
Conc: 0.40 ug/ml