

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG082118\
 Data File : FG002158.D
 Signal(s) : FID1A.ch
 Acq On : 21 Aug 2018 23:00
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 22 02:00:22 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG073018.M
 Quant Title :
 QLast Update : Mon Jul 30 13:56:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.456	2095210	16.622 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.352	32113	0.259 ug/ml
15) N-TETRATRIACONTANE	19.136	104838	0.964 ug/ml
16) N-HEXATRIACONTANE	19.886	64033	0.667 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG082118\
Data File : FG002158.D
Signal(s) : FID1A.ch
Acq On : 21 Aug 2018 23:00
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 22 02:00:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG073018.M
Quant Title :
QLast Update : Mon Jul 30 13:56:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

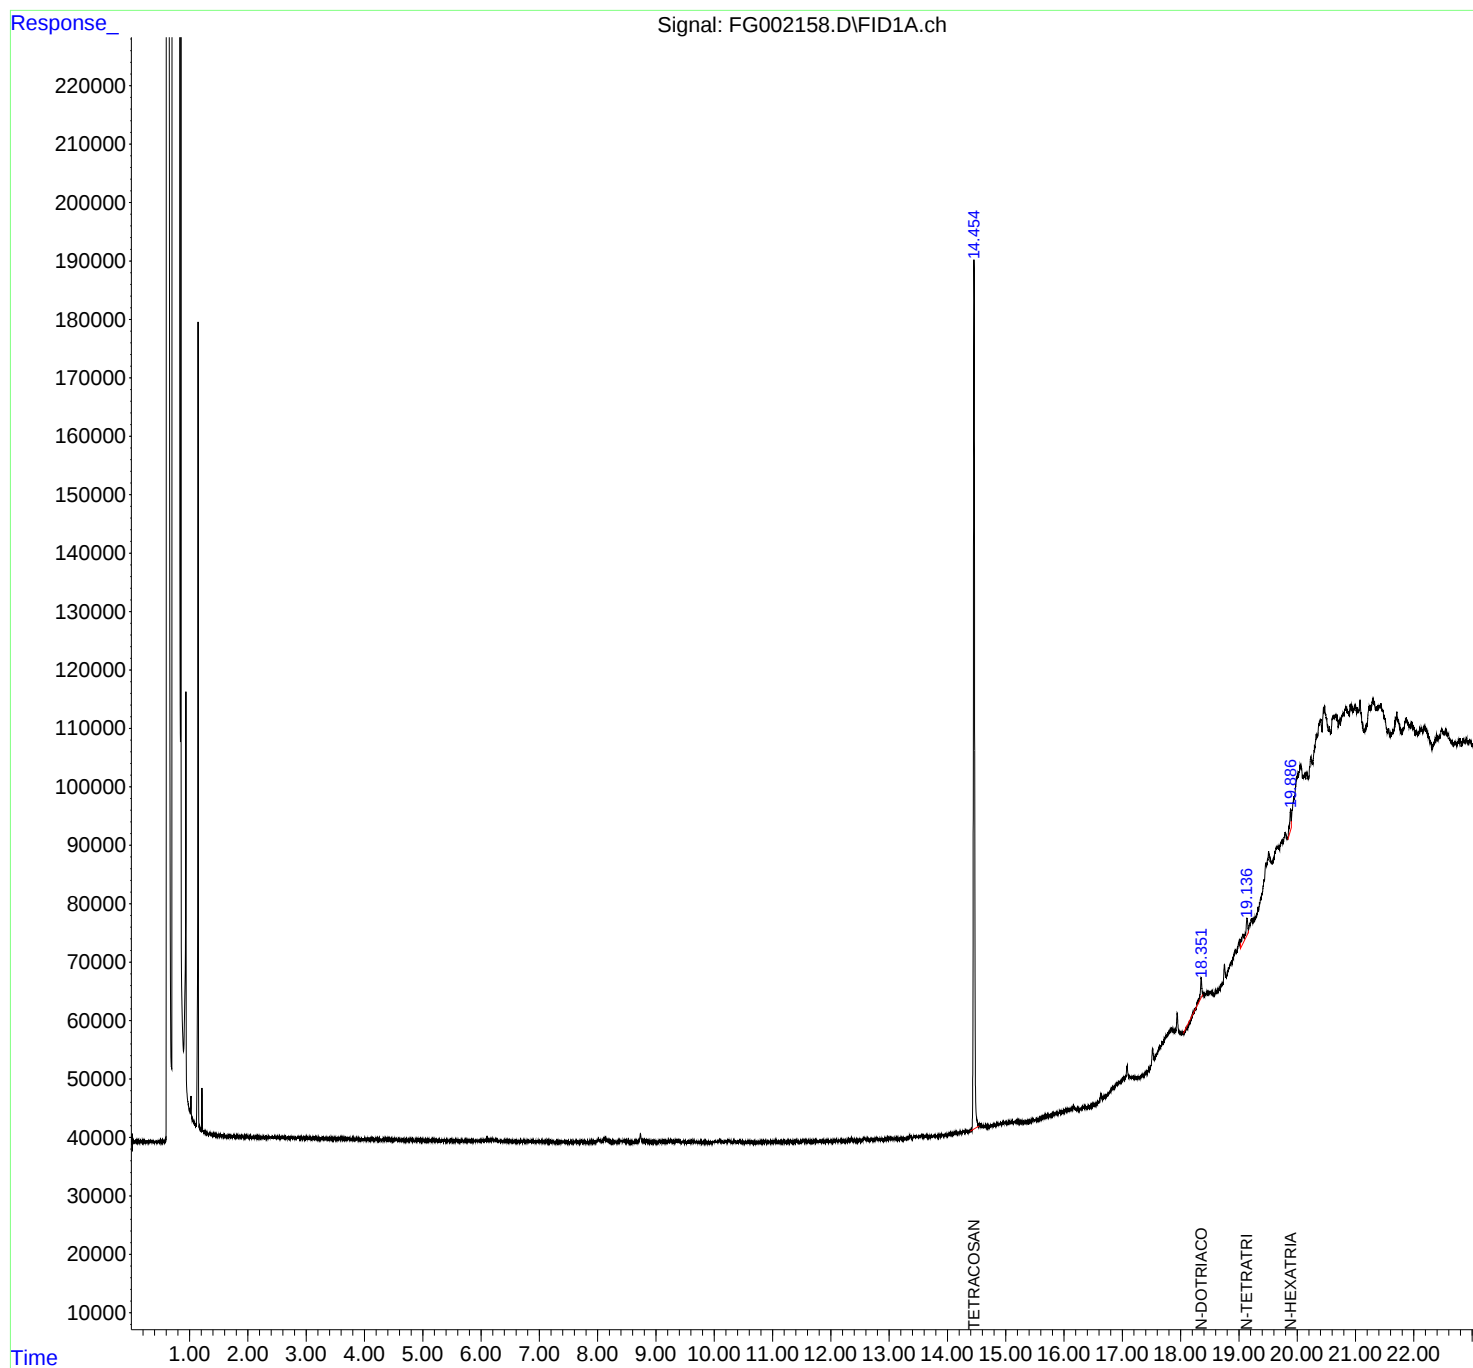


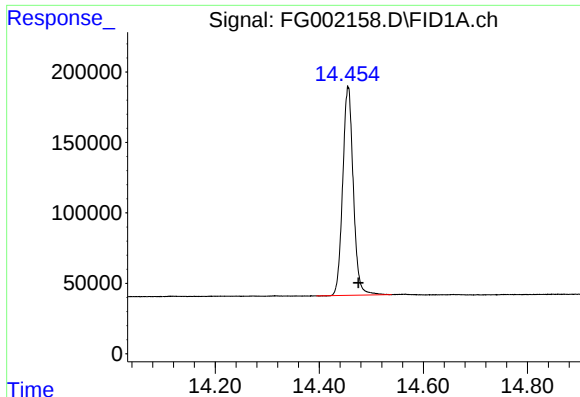

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.456 min
Delta R.T.: -0.020 min
Response: 2095210
Conc: 16.62 ug/ml

Instrument :
FID_G
ClientSampleId :

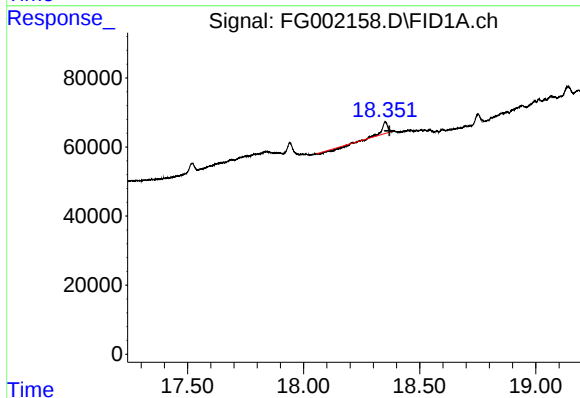


#14 N-DOTRIACONTANE

R.T.: 18.352 min
Delta R.T.: -0.018 min
Response: 32113
Conc: 0.26 ug/ml

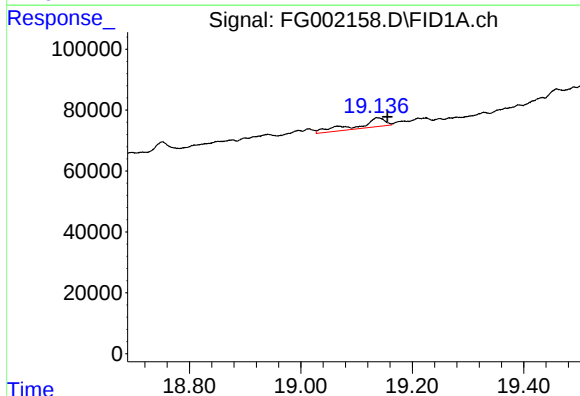

#15 N-TETRATRIACONTANE

R.T.: 19.136 min
Delta R.T.: -0.019 min
Response: 104838
Conc: 0.96 ug/ml

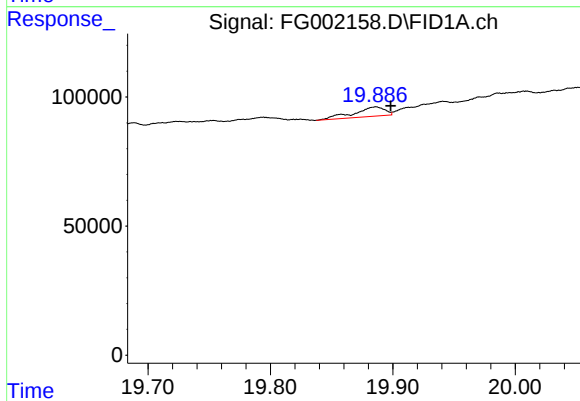

#16 N-HEXATRIACONTANE

R.T.: 19.886 min
Delta R.T.: -0.013 min
Response: 64033
Conc: 0.67 ug/ml