

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG082118\
Data File : FG002145.D
Signal(s) : FID1A.ch
Acq On : 21 Aug 2018 15:51
Operator : AJ\SJ
Sample : J4553-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
EPE-P-9(20-22)

Integration File: autoint1.e
Quant Time: Aug 22 01:57:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG073018.M
Quant Title :
QLast Update : Mon Jul 30 13:56:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.457	3008508	23.867 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG082118\
Data File : FG002145.D
Signal(s) : FID1A.ch
Acq On : 21 Aug 2018 15:51
Operator : AJ\SJ
Sample : J4553-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
EPE-P-9(20-22)

Integration File: autoint1.e
Quant Time: Aug 22 01:57:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG073018.M
Quant Title :
QLast Update : Mon Jul 30 13:56:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

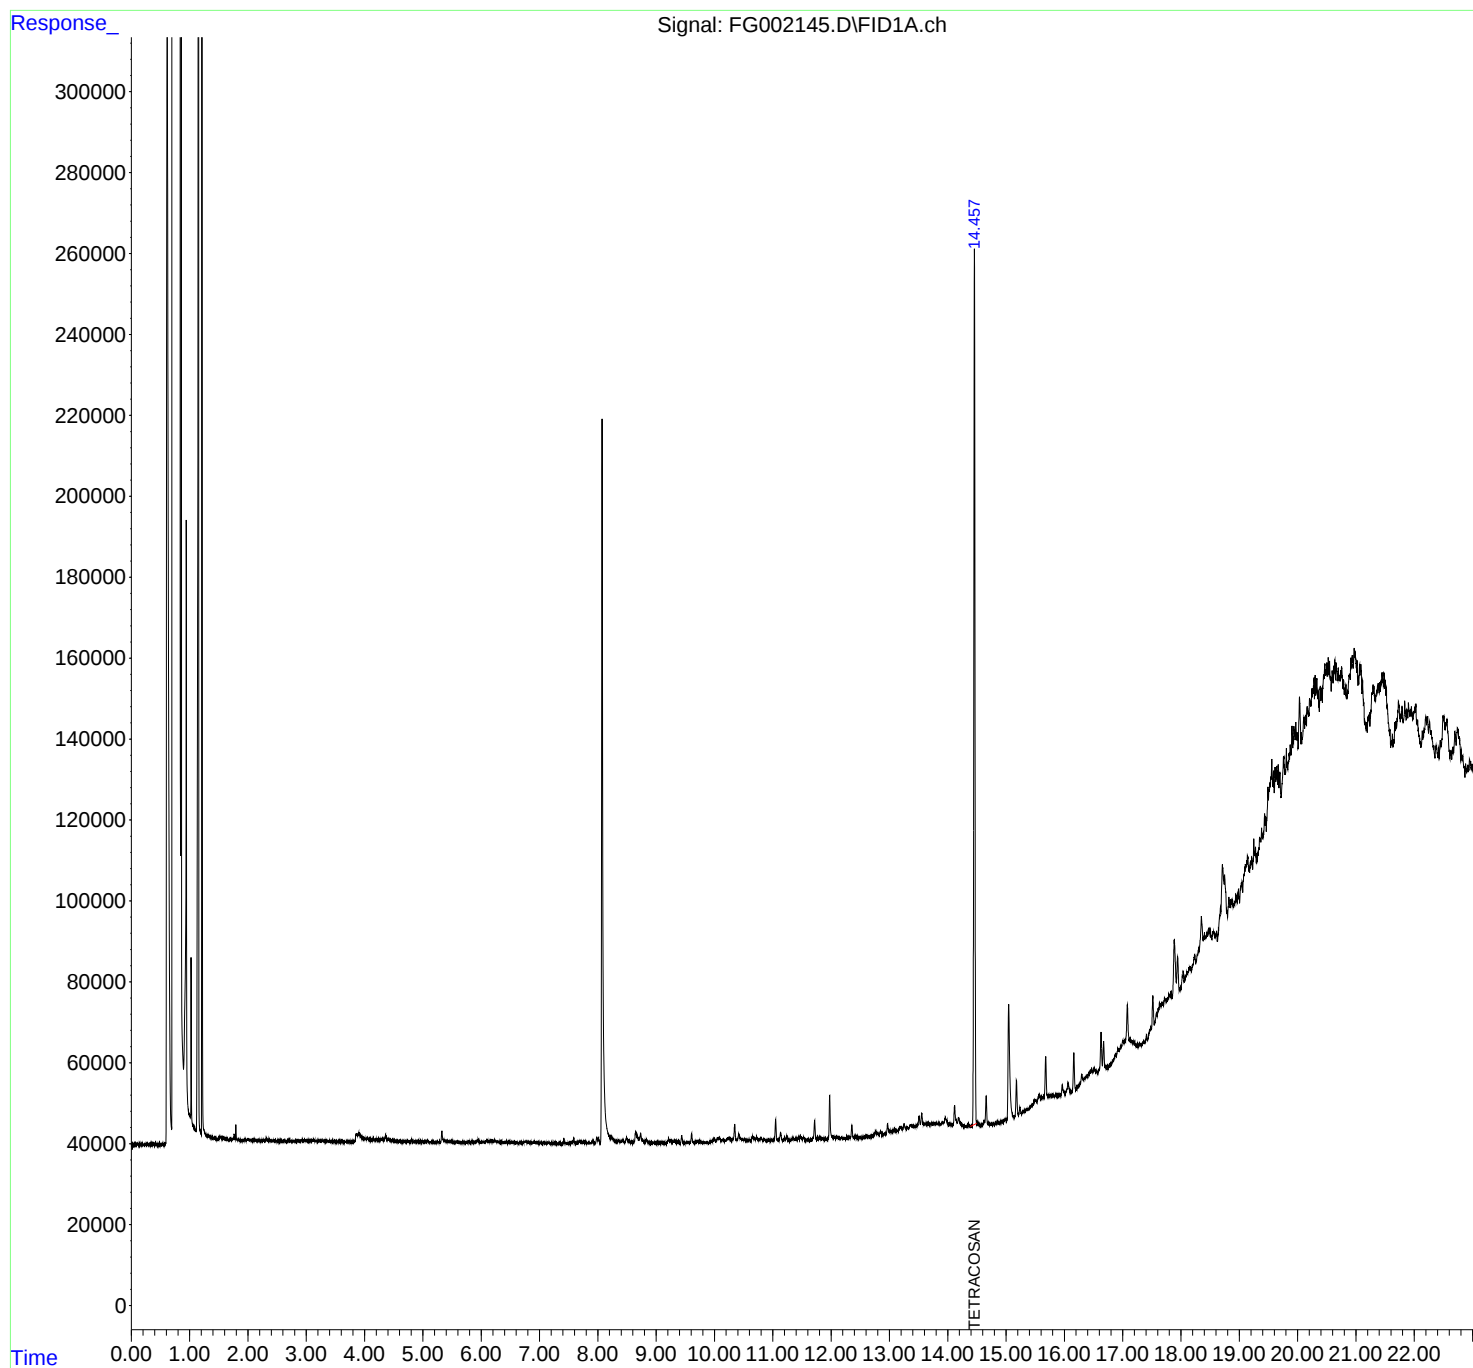

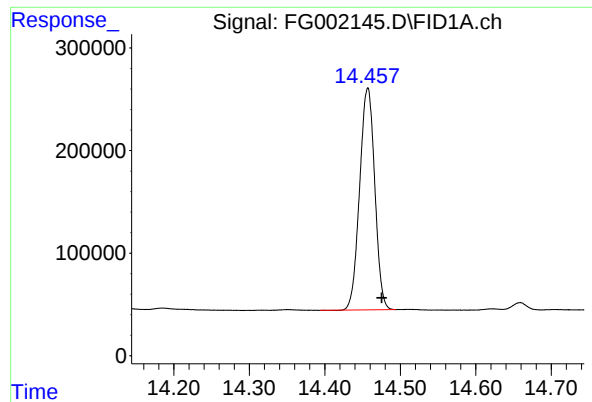

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.457 min
Delta R.T.: -0.019 min
Response: 3008508
Conc: 23.87 ug/ml

Instrument :
FID_G
ClientSampleId :
EPE-P-9(20-22)