

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG082119\
Data File : FG005665.D
Signal(s) : FID1A.ch
Acq On : 21 Aug 2019 12:37
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 22 07:26:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080819.M
Quant Title :
QLast Update : Thu Aug 08 16:03:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.477	4490670	30.654 ug/ml
10)	N-TETRACOSANE	14.946	35833	0.247 ug/ml
11)	N-HEXACOSANE	15.975	35120	0.245 ug/ml
12)	N-OCTACOSANE	16.930	3704548	24.506 ug/ml
13)	N-TRIACONTANE	17.817	110213	0.729 ug/ml
14)	N-DOTRIACONTANE	18.652	132402	0.989 ug/ml
15)	N-TETRATRIACONTANE	19.438	93230	0.755 ug/ml
16)	N-HEXATRIACONTANE	20.183	287309	2.492 ug/ml
17)	N-OCTATRIACONTANE	20.939	32471	0.311 ug/ml
18)	N-TETRACONTANE	21.886	51916	0.499 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG082119\
Data File : FG005665.D
Signal(s) : FID1A.ch
Acq On : 21 Aug 2019 12:37
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 22 07:26:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080819.M
Quant Title :
QLast Update : Thu Aug 08 16:03:53 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

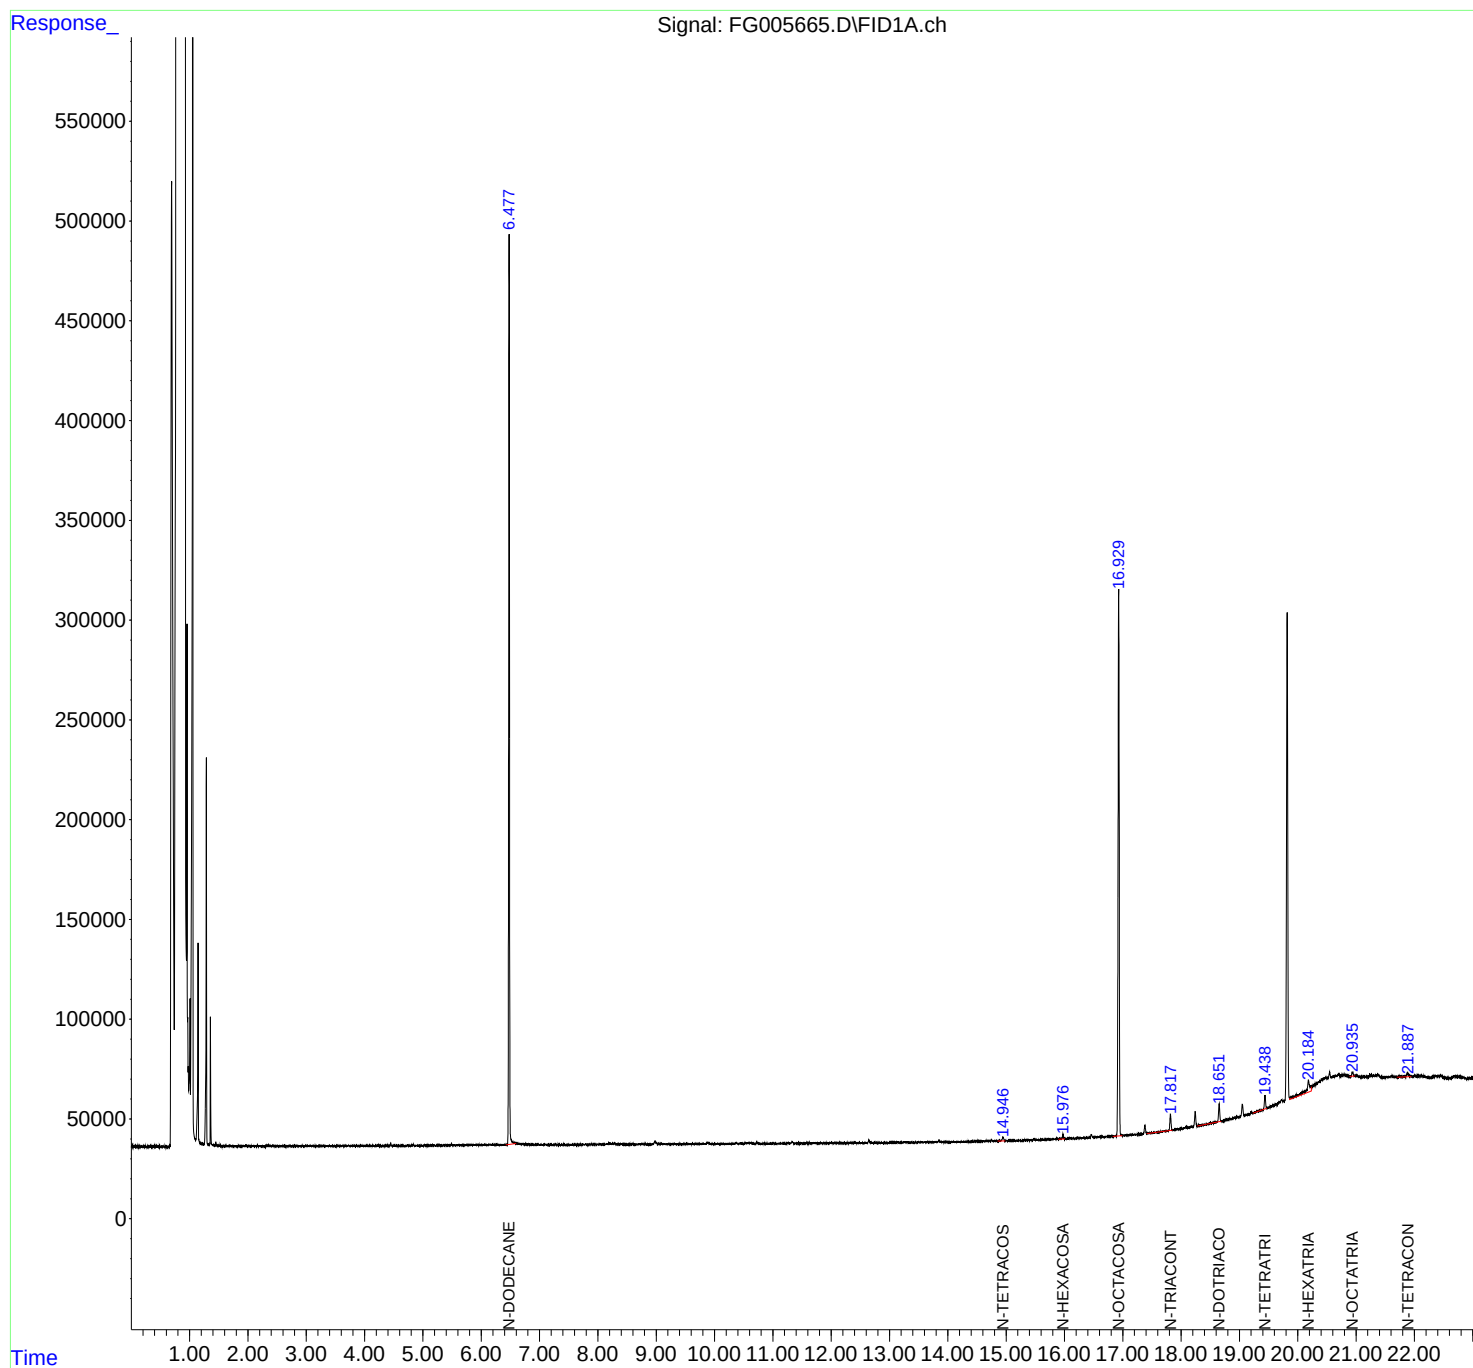

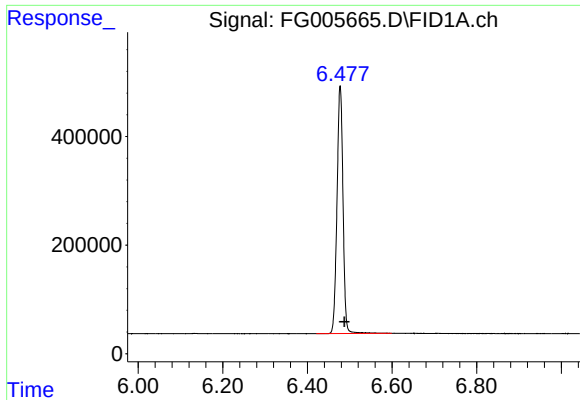


#3 N-DODECANE

R.T.: 6.477 min
Delta R.T.: -0.010 min
Response: 4490670
Conc: 30.65 ug/ml

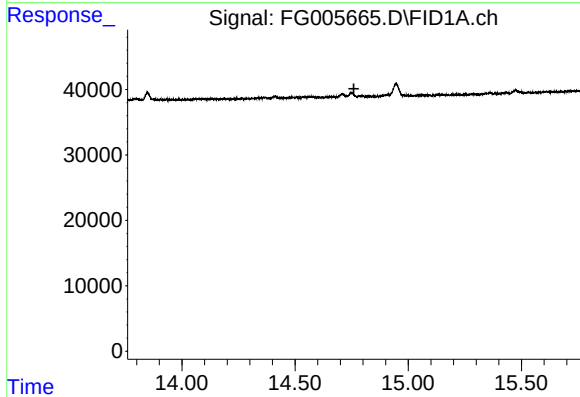


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.760 min
Response: 0
Conc: N.D.

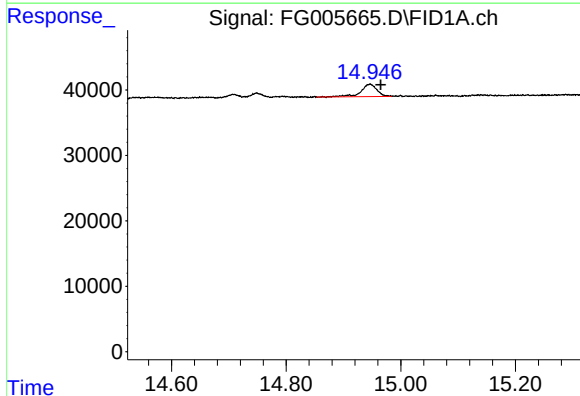


#10 N-TETRACOSANE

R.T.: 14.946 min
Delta R.T.: -0.019 min
Response: 35833
Conc: 0.25 ug/ml

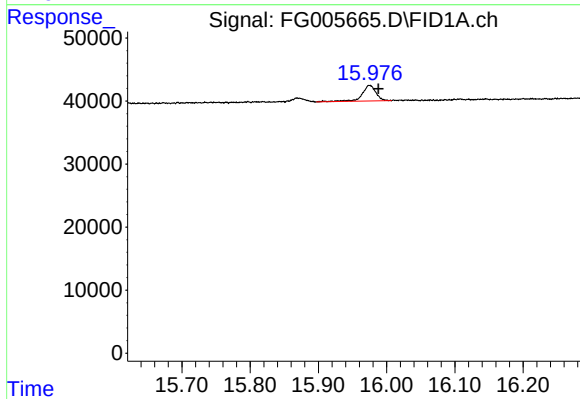


#11 N-HEXACOSANE

R.T.: 15.975 min
Delta R.T.: -0.013 min
Response: 35120
Conc: 0.24 ug/ml

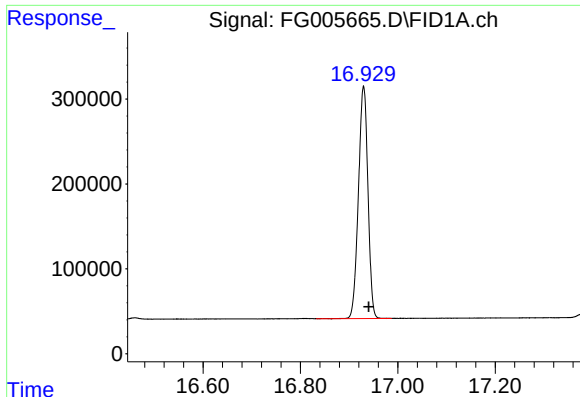


#12 N-OCTACOSANE

R.T.: 16.930 min
Delta R.T.: -0.010 min
Response: 3704548
Conc: 24.51 ug/ml

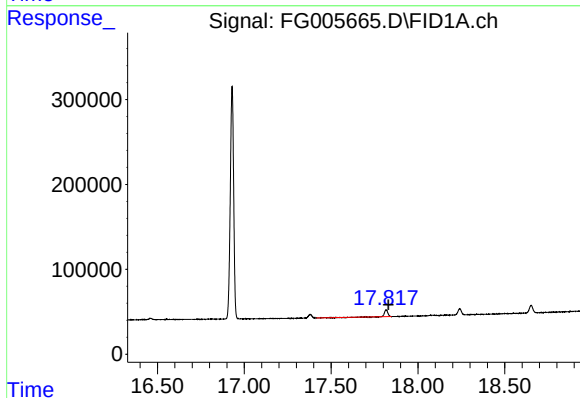


#13 N-TRIACONTANE

R.T.: 17.817 min
Delta R.T.: -0.012 min
Response: 110213
Conc: 0.73 ug/ml

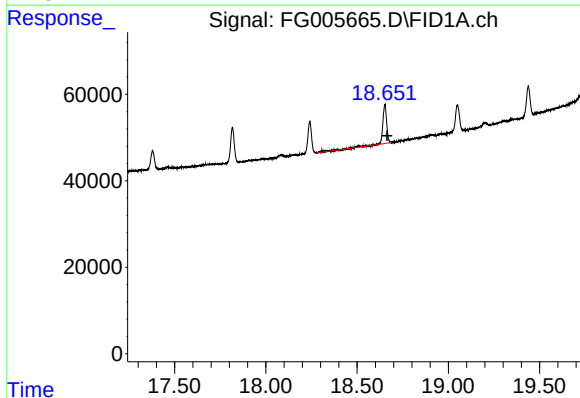


#14 N-DOTRIACONTANE

R.T.: 18.652 min
Delta R.T.: -0.012 min
Response: 132402
Conc: 0.99 ug/ml

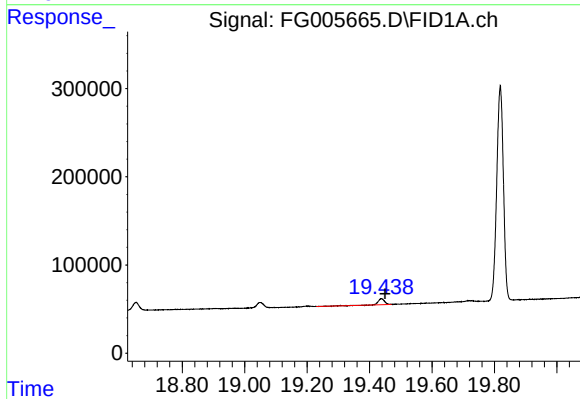


#15 N-TETRATRIACONTANE

R.T.: 19.438 min
Delta R.T.: -0.012 min
Response: 93230
Conc: 0.75 ug/ml

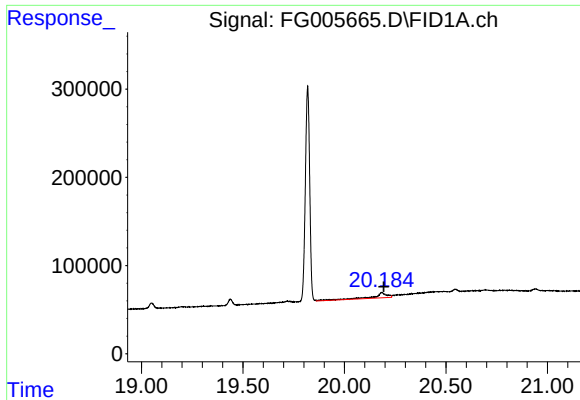


#16 N-HEXATRIACONTANE

R.T.: 20.183 min
Delta R.T.: -0.010 min
Response: 287309
Conc: 2.49 ug/ml

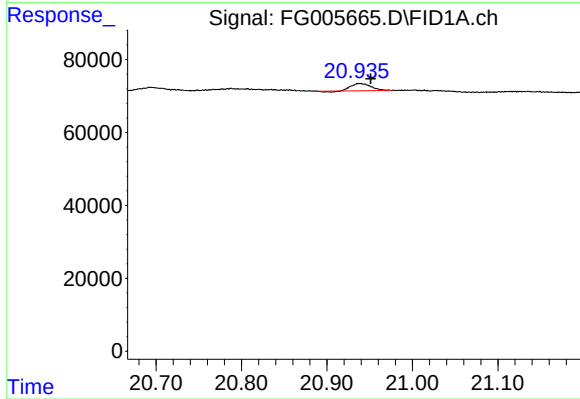

#17 N-OCTATRIACONTANE

R.T.: 20.939 min
Delta R.T.: -0.012 min
Response: 32471
Conc: 0.31 ug/ml

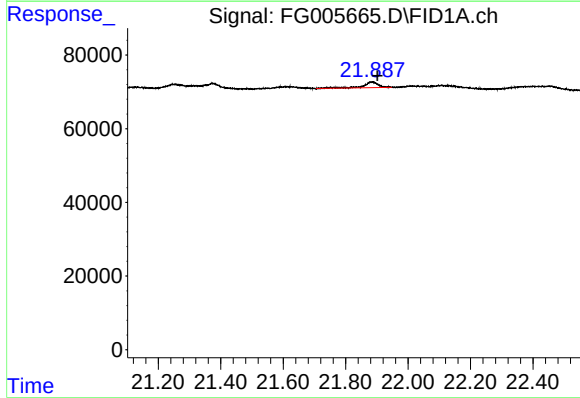

#18 N-TETRACONTANE

R.T.: 21.886 min
Delta R.T.: -0.016 min
Response: 51916
Conc: 0.50 ug/ml