

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG082123\
Data File : FG012752.D
Signal(s) : FID1A.ch
Acq On : 21 Aug 2023 18:40
Operator : YP\AJ
Sample : 04089-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
BU-3-081823

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/22/2023
Supervised By :Ankita Jodhani 08/22/2023

Integration File: autoint1.e
Quant Time: Aug 21 23:54:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080223.M
Quant Title :
QLast Update : Wed Aug 02 18:57:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.090	2459179	21.983 ug/mlm

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG082123\
Data File : FG012752.D
Signal(s) : FID1A.ch
Acq On : 21 Aug 2023 18:40
Operator : YP\AJ
Sample : 04089-01
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
BU-3-081823


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/22/2023
Supervised By :Ankita Jodhani 08/22/2023

Integration File: autoint1.e
Quant Time: Aug 21 23:54:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080223.M
Quant Title :
QLast Update : Wed Aug 02 18:57:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

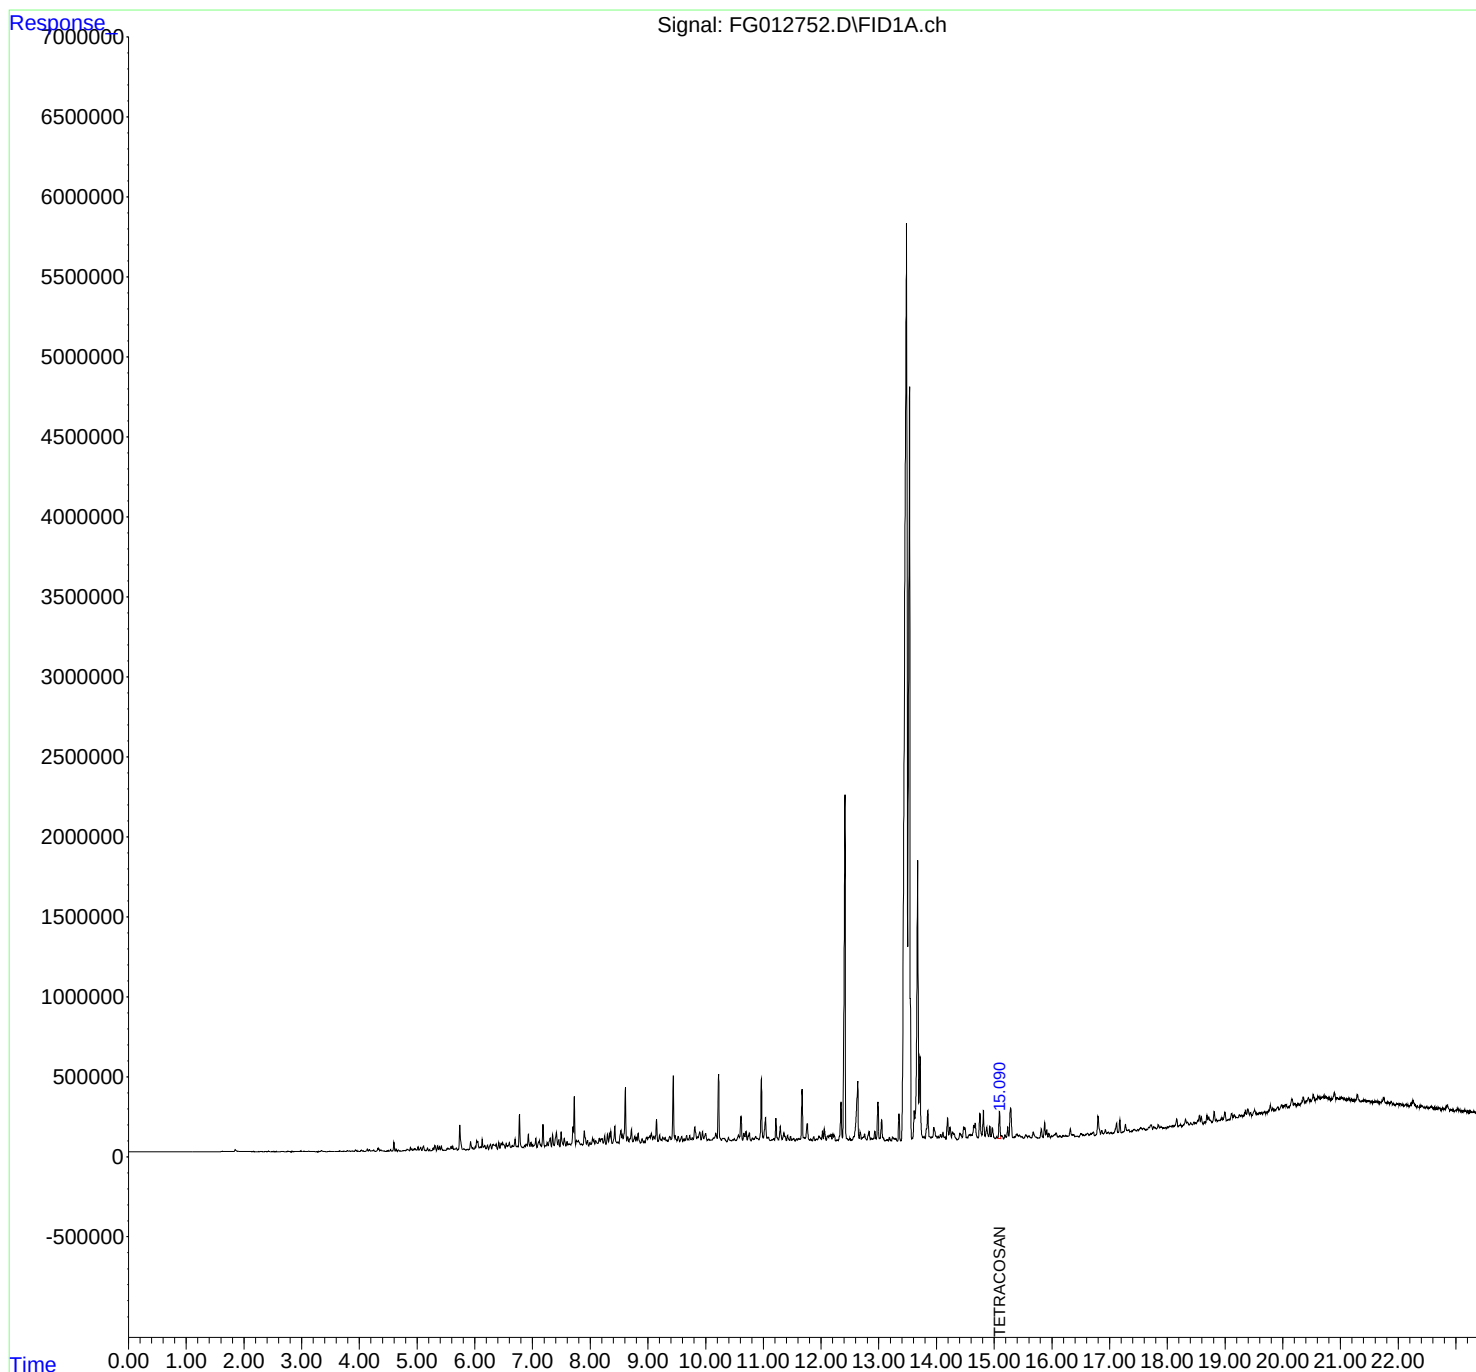

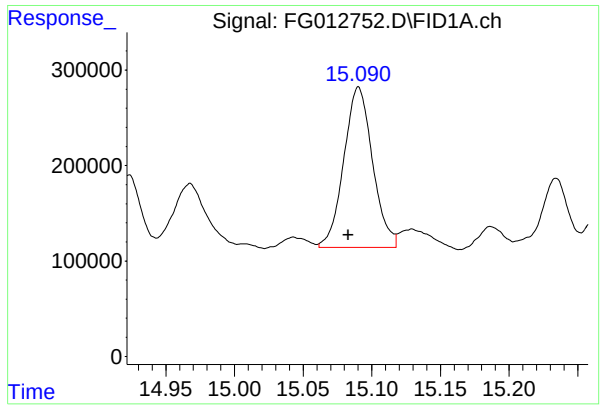

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.090 min
Delta R.T.: 0.007 min
Response: 2459179
Conc: 21.98 ug/ml

Instrument :

FID_G

ClientSampleId :

BU-3-081823

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 08/22/2023

Supervised By :Ankita Jodhani 08/22/2023