

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG082124\
 Data File : FG014136.D
 Signal(s) : FID1A.ch
 Acq On : 21 Aug 2024 15:16
 Operator : YP\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 50 PPM TRPH STD

Integration File: autoint1.e
 Quant Time: Aug 22 02:06:40 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG081624.M
 Quant Title :
 QLast Update : Fri Aug 16 10:59:42 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.935	5467504	51.739 ug/ml
Target Compounds			
2) N-DECANE	4.454	5746520	57.691 ug/ml
3) N-DODECANE	6.628	5893493	57.383 ug/ml
4) N-TETRADECANE	8.460	5842434	53.494 ug/ml
5) N-HEXADECANE	10.071	6112761	54.552 ug/ml
6) N-OCTADECANE	11.518	6218040	53.328 ug/ml
7) N-EICOSANE	12.831	6340162	53.270 ug/ml
8) N-DOCOSANE	14.033	6150757	52.447 ug/ml
10) N-TETRACOSANE	15.139	6079939	51.441 ug/ml
11) N-HEXACOSANE	16.163	6048072	51.086 ug/ml
12) N-OCTACOSANE	17.114	5979435	50.721 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG082124\
Data File : FG014136.D
Signal(s) : FID1A.ch
Acq On : 21 Aug 2024 15:16
Operator : YP\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

Integration File: autoint1.e
Quant Time: Aug 22 02:06:40 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG081624.M
Quant Title :
QLast Update : Fri Aug 16 10:59:42 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

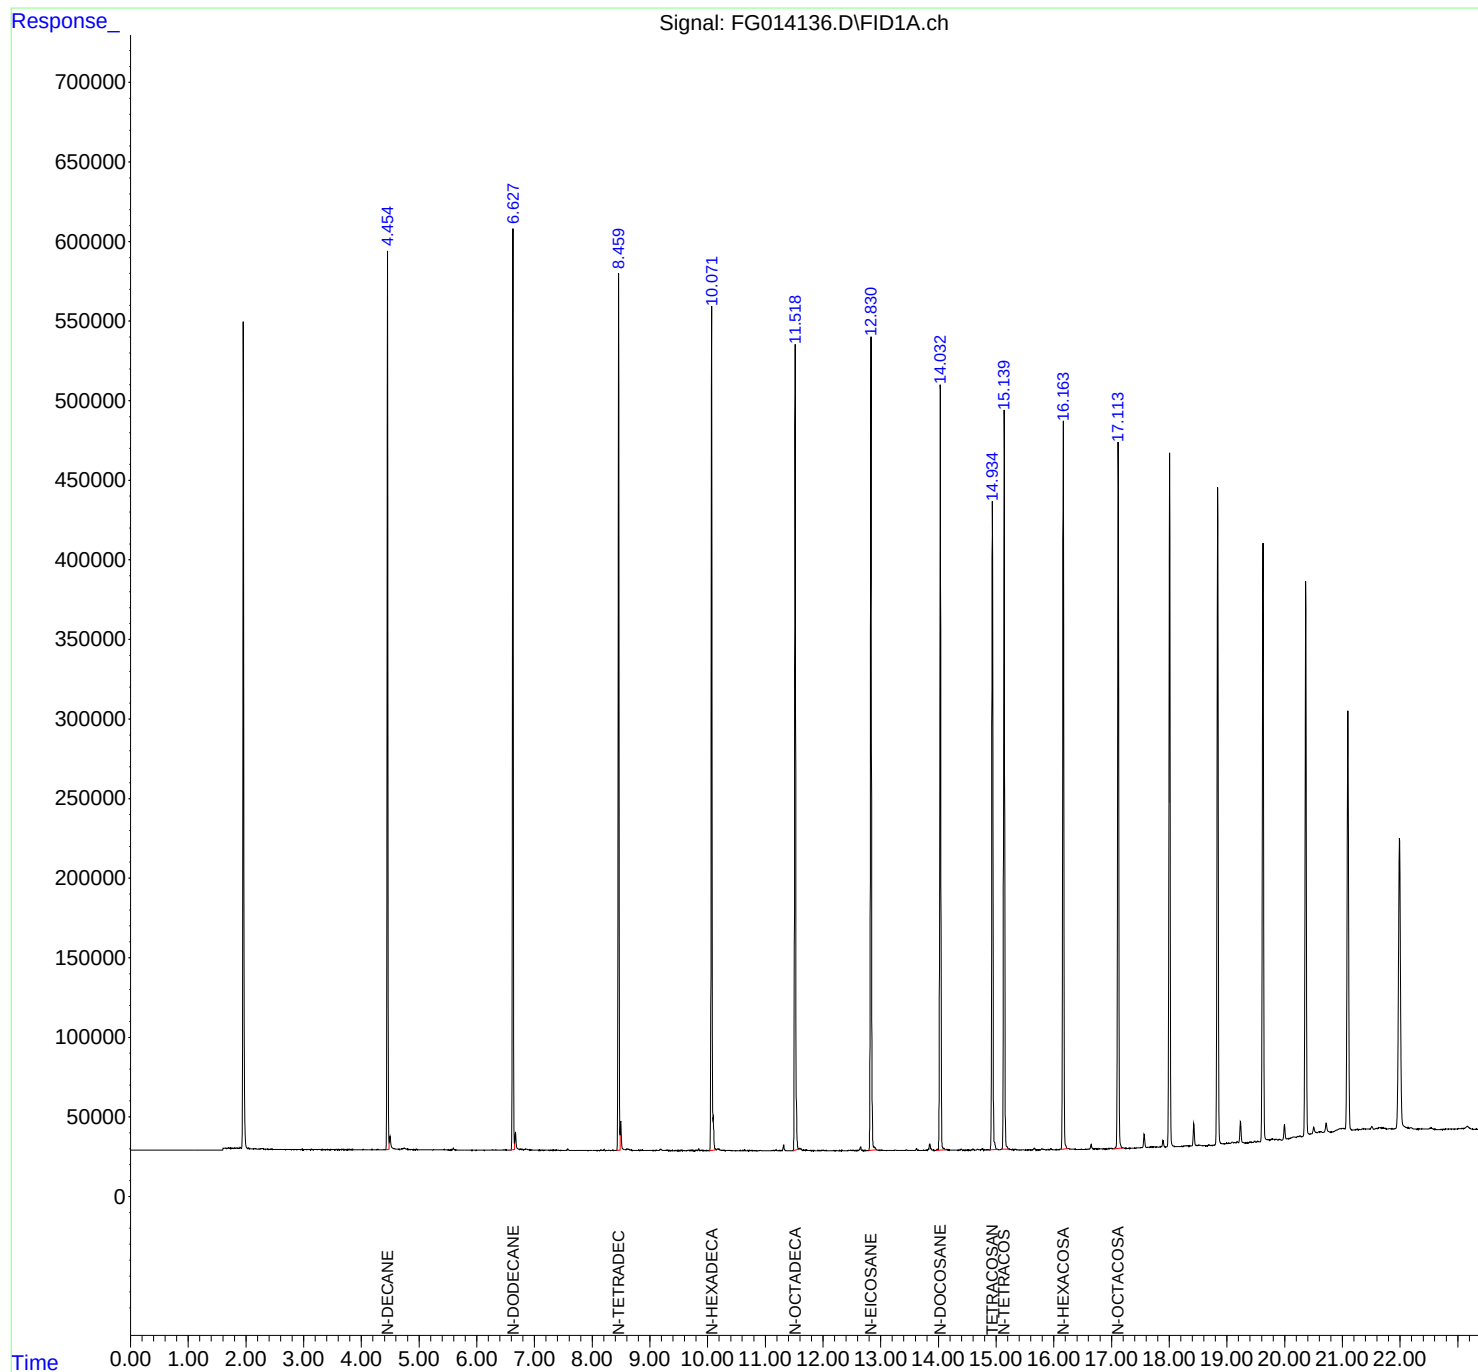


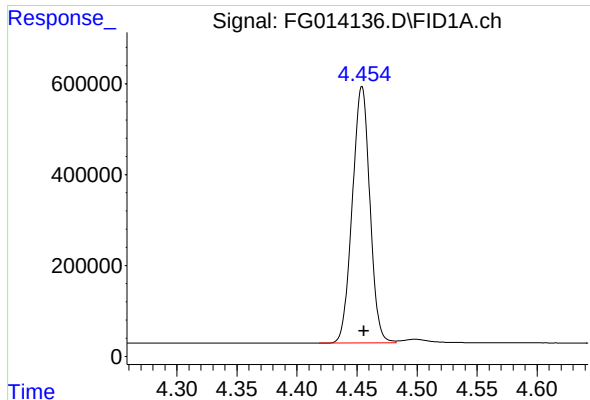

#2 N-DECANE


R.T.: 4.454 min
Delta R.T.: -0.002 min
Response: 5746520
Conc: 57.69 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

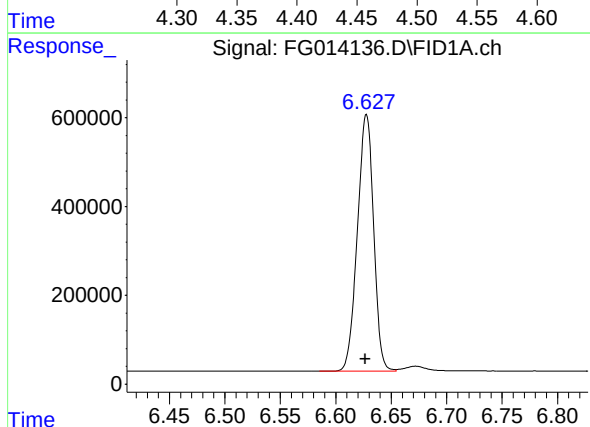


#3 N-DODECANE

R.T.: 6.628 min
Delta R.T.: 0.000 min
Response: 5893493
Conc: 57.38 ug/ml

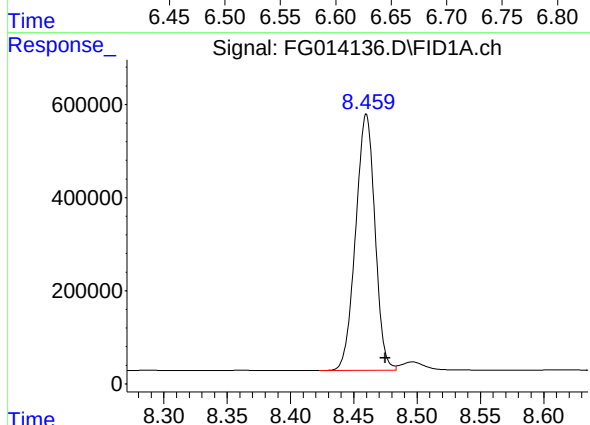


#4 N-TETRADECANE

R.T.: 8.460 min
Delta R.T.: -0.015 min
Response: 5842434
Conc: 53.49 ug/ml

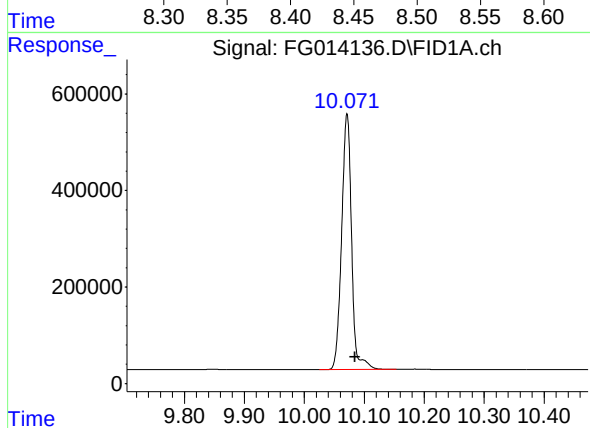

#5 N-HEXADECANE


R.T.: 10.071 min
Delta R.T.: -0.013 min
Response: 6112761
Conc: 54.55 ug/ml

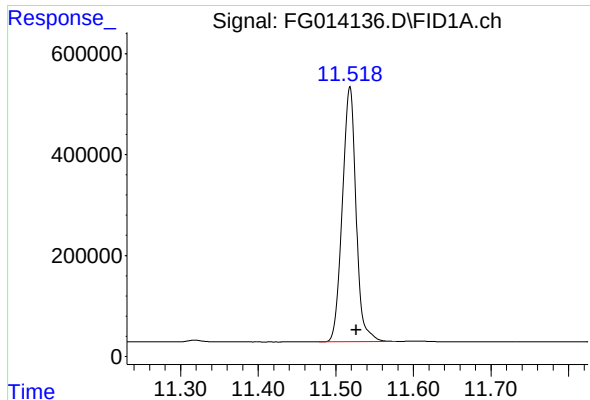

#6 N-OCTADECANE


R.T.: 11.518 min
Delta R.T.: -0.008 min
Response: 6218040
Conc: 53.33 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

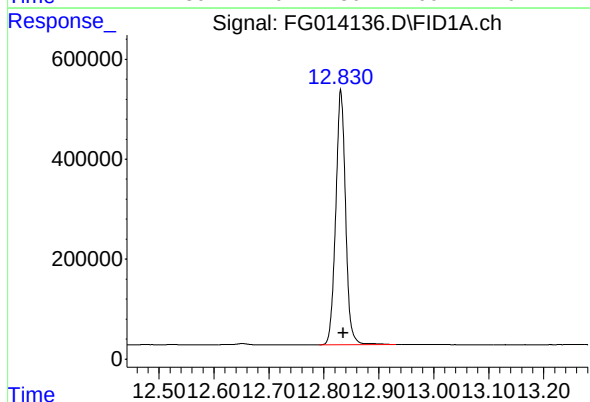


#7 N-EICOSANE

R.T.: 12.831 min
Delta R.T.: -0.005 min
Response: 6340162
Conc: 53.27 ug/ml

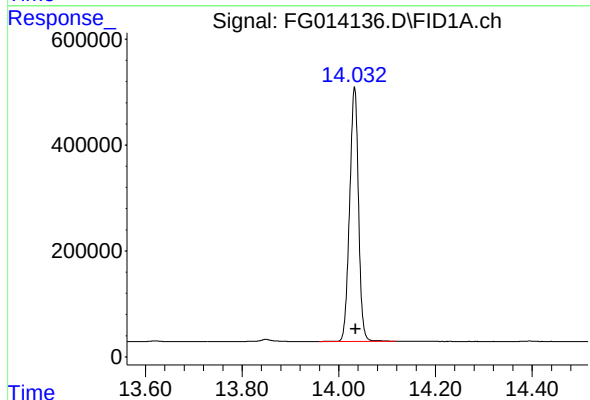


#8 N-DOCOSANE

R.T.: 14.033 min
Delta R.T.: -0.002 min
Response: 6150757
Conc: 52.45 ug/ml

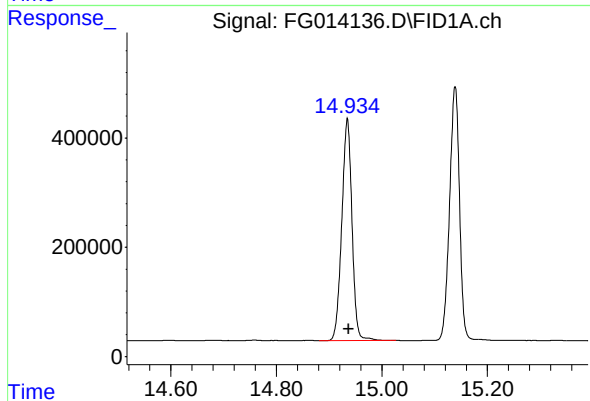

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.935 min
Delta R.T.: -0.002 min
Response: 5467504
Conc: 51.74 ug/ml

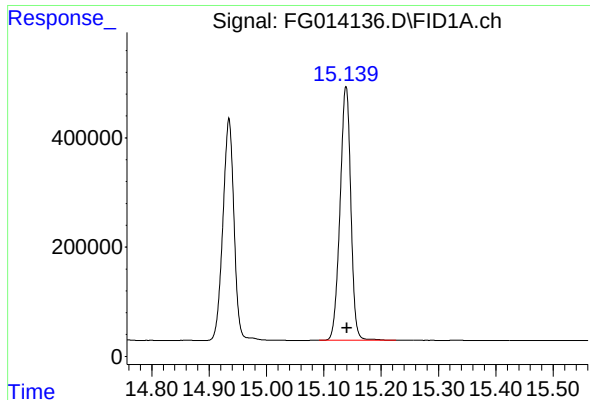

#10 N-TETRACOSANE


R.T.: 15.139 min
Delta R.T.: -0.001 min
Response: 6079939
Conc: 51.44 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

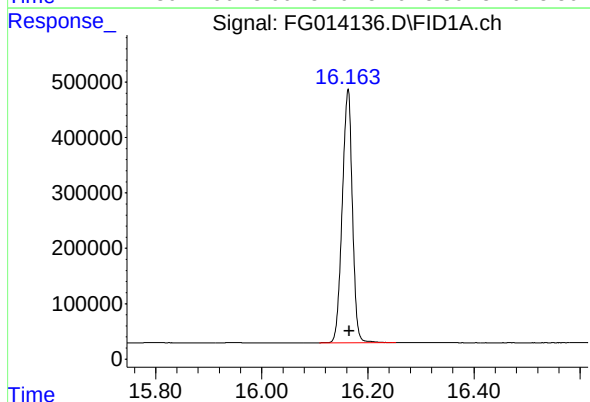

#11 N-HEXACOSANE

R.T.: 16.163 min
Delta R.T.: -0.002 min
Response: 6048072
Conc: 51.09 ug/ml

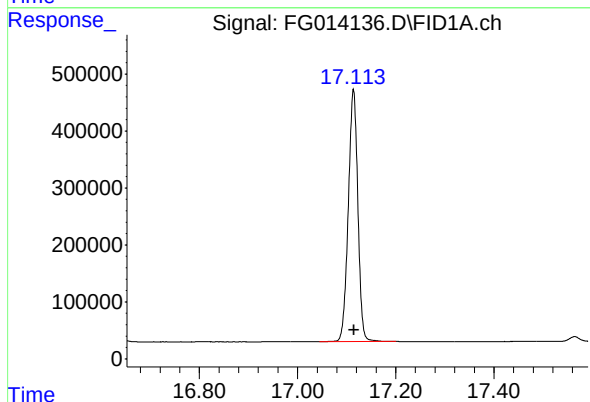

#12 N-OCTACOSANE

R.T.: 17.114 min
Delta R.T.: 0.000 min
Response: 5979435
Conc: 50.72 ug/ml