

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG082218\
Data File : FG002163.D
Signal(s) : FID1A.ch
Acq On : 22 Aug 2018 13:46
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 23 08:54:48 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG073018.M
Quant Title :
QLast Update : Mon Jul 30 13:56:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.218	4247461	28.273 ug/ml
12)	N-OCTACOSANE	16.634	4018375	28.803 ug/ml
13)	N-TRIACONTANE	17.521	289008	2.116 ug/ml
14)	N-DOTRIACONTANE	18.354	354937	2.866 ug/ml
15)	N-TETRATRIACONTANE	19.140	244639	2.250 ug/ml
16)	N-HEXATRIACONTANE	19.884	142912	1.488 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG082218\
Data File : FG002163.D
Signal(s) : FID1A.ch
Acq On : 22 Aug 2018 13:46
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 23 08:54:48 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG073018.M
Quant Title :
QLast Update : Mon Jul 30 13:56:56 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

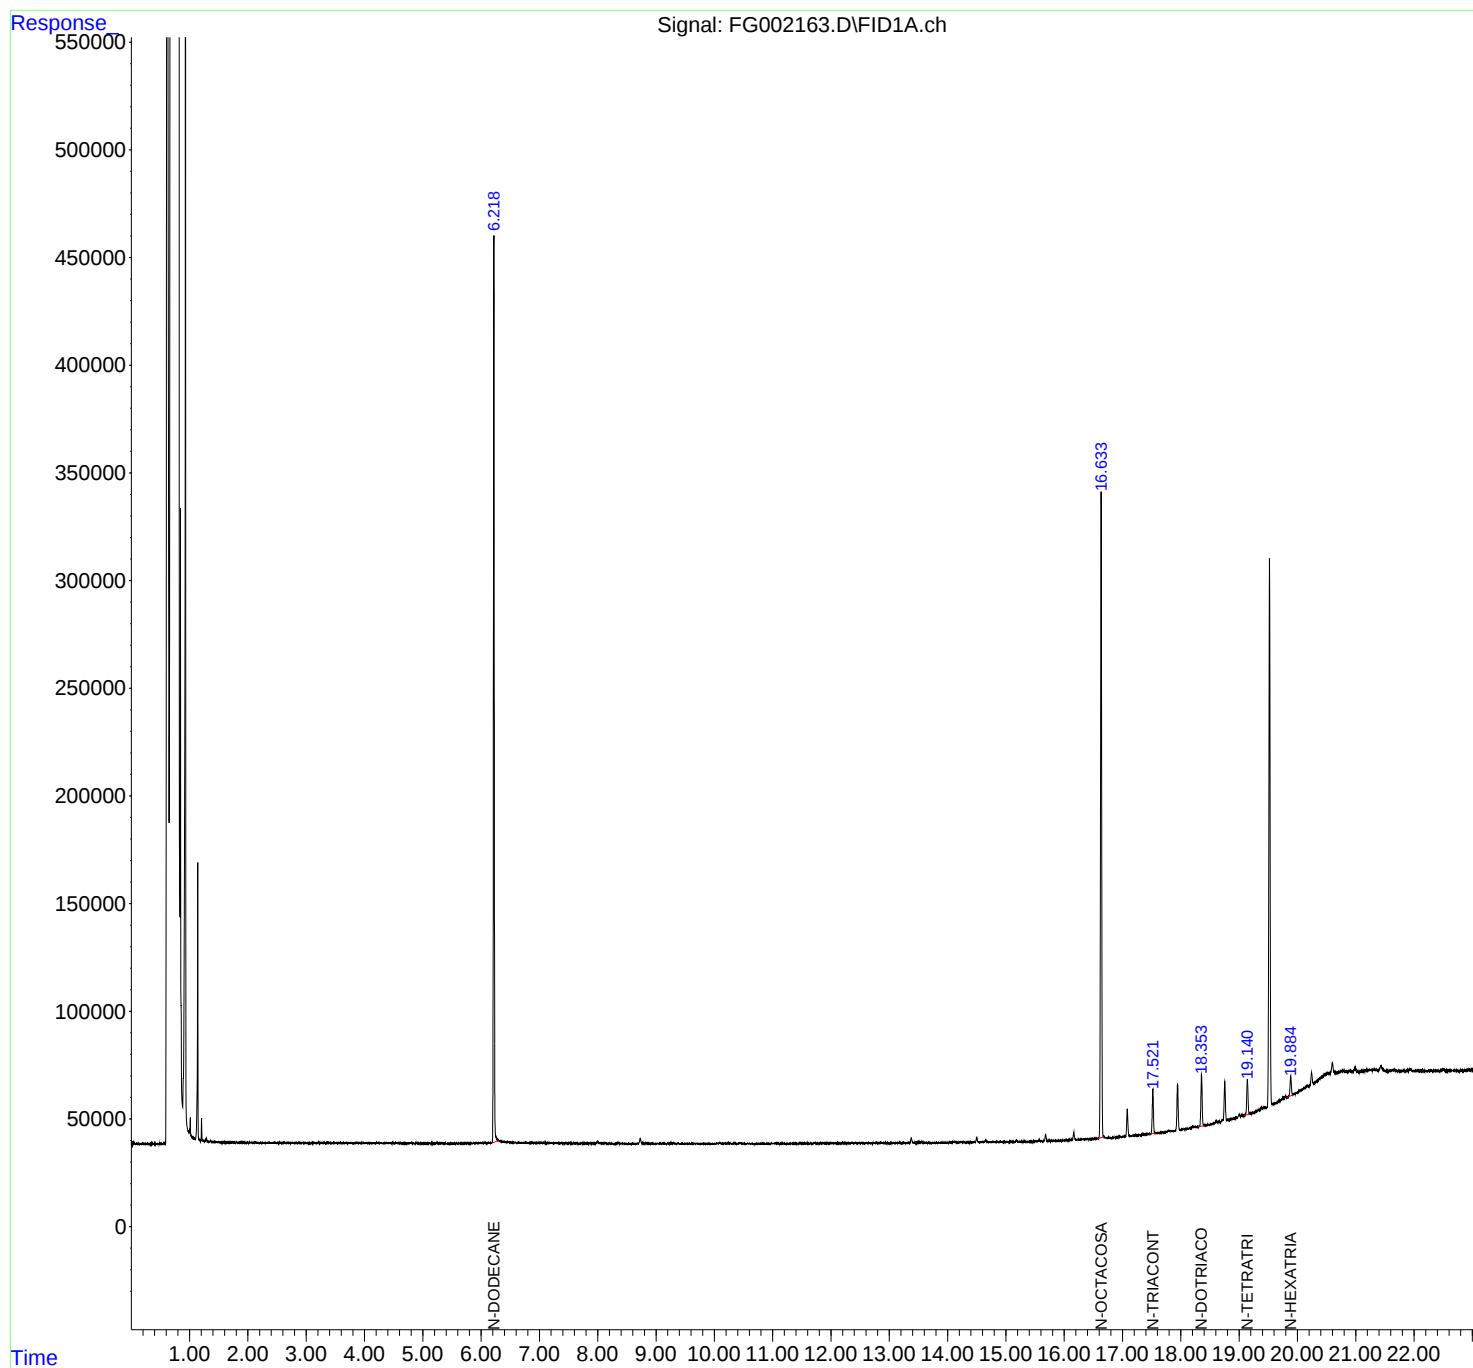


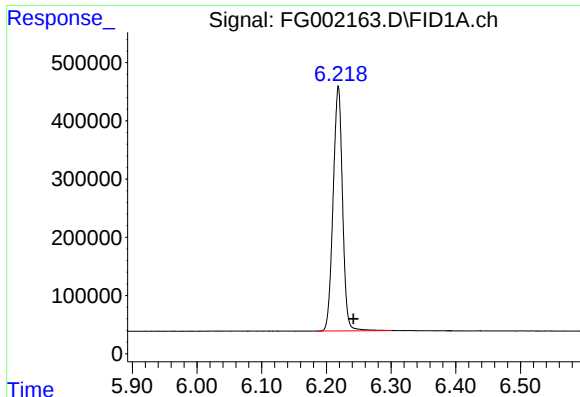

#3 N-DODECANE


R.T.: 6.218 min
Delta R.T.: -0.023 min
Response: 4247461
Conc: 28.27 ug/ml

Instrument :
FID_G
ClientSampleId :

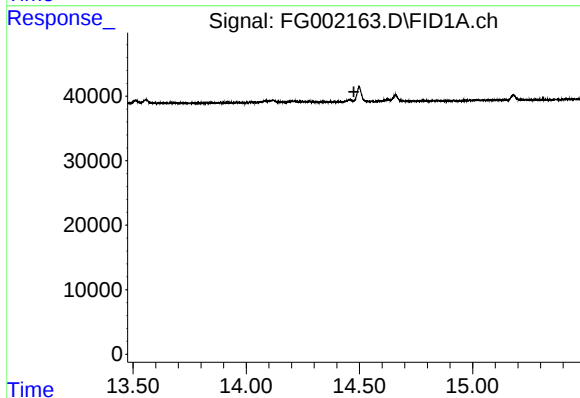


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.475 min
Response: 0
Conc: N.D.

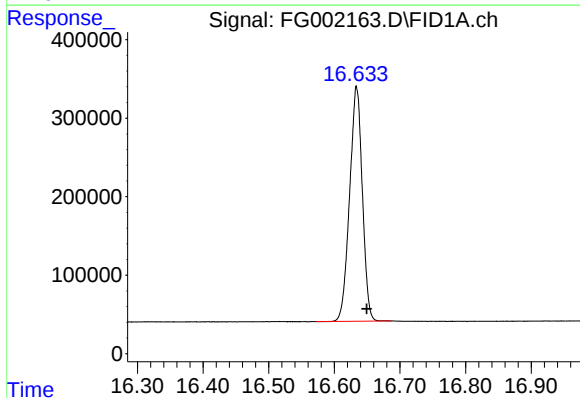


#12 N-OCTACOSANE

R.T.: 16.634 min
Delta R.T.: -0.016 min
Response: 4018375
Conc: 28.80 ug/ml

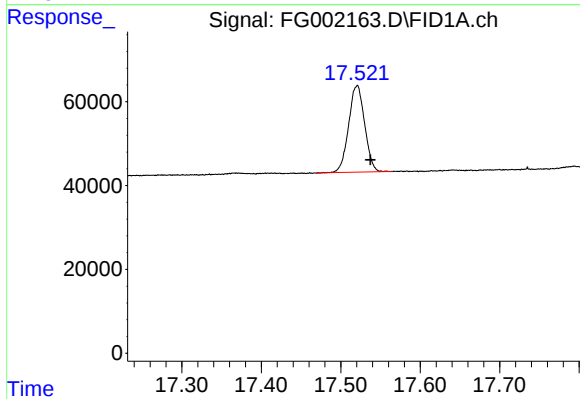

#13 N-TRIACONTANE


R.T.: 17.521 min
Delta R.T.: -0.017 min
Response: 289008
Conc: 2.12 ug/ml

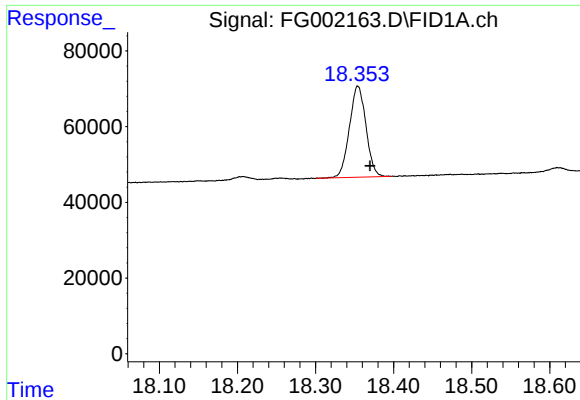

#14 N-DOTRIACONTANE


R.T.: 18.354 min
Delta R.T.: -0.016 min
Response: 354937
Conc: 2.87 ug/ml

Instrument :
FID_G
ClientSampleId :

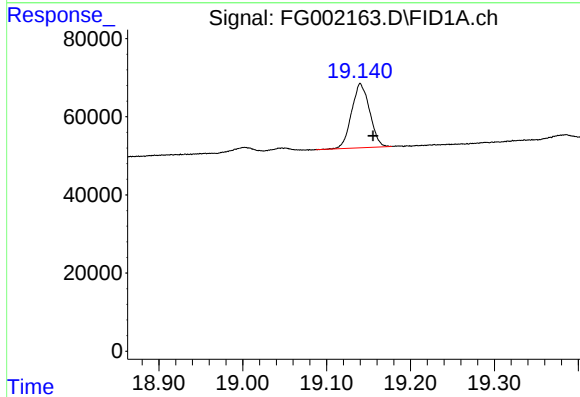

#15 N-TETRATRIACONTANE

R.T.: 19.140 min
Delta R.T.: -0.015 min
Response: 244639
Conc: 2.25 ug/ml

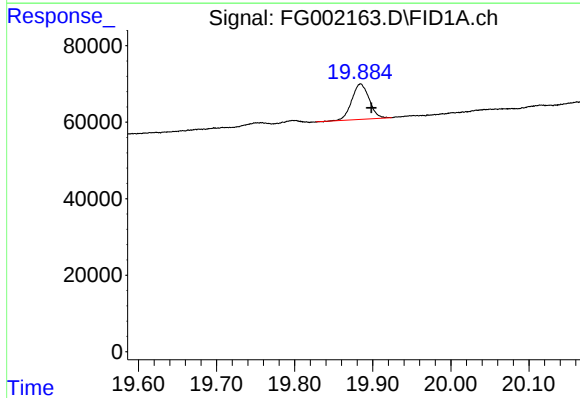

#16 N-HEXATRIACONTANE

R.T.: 19.884 min
Delta R.T.: -0.014 min
Response: 142912
Conc: 1.49 ug/ml