

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG082222\
Data File : FG010403.D
Signal(s) : FID1A.ch
Acq On : 22 Aug 2022 13:06
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 23 01:49:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG072822.M
Quant Title :
QLast Update : Thu Jul 28 15:10:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.499	3719750	27.062 ug/ml
12)	N-OCTACOSANE	16.968	3399034	24.617 ug/ml
13)	N-TRIACONTANE	17.855	68596	0.506 ug/ml
14)	N-DOTRIACONTANE	18.686	96915	0.738 ug/ml
15)	N-TETRATRIACONTANE	19.471	95971	0.767 ug/ml
16)	N-HEXATRIACONTANE	20.212	73659	0.639 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG082222\
Data File : FG010403.D
Signal(s) : FID1A.ch
Acq On : 22 Aug 2022 13:06
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 23 01:49:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG072822.M
Quant Title :
QLast Update : Thu Jul 28 15:10:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

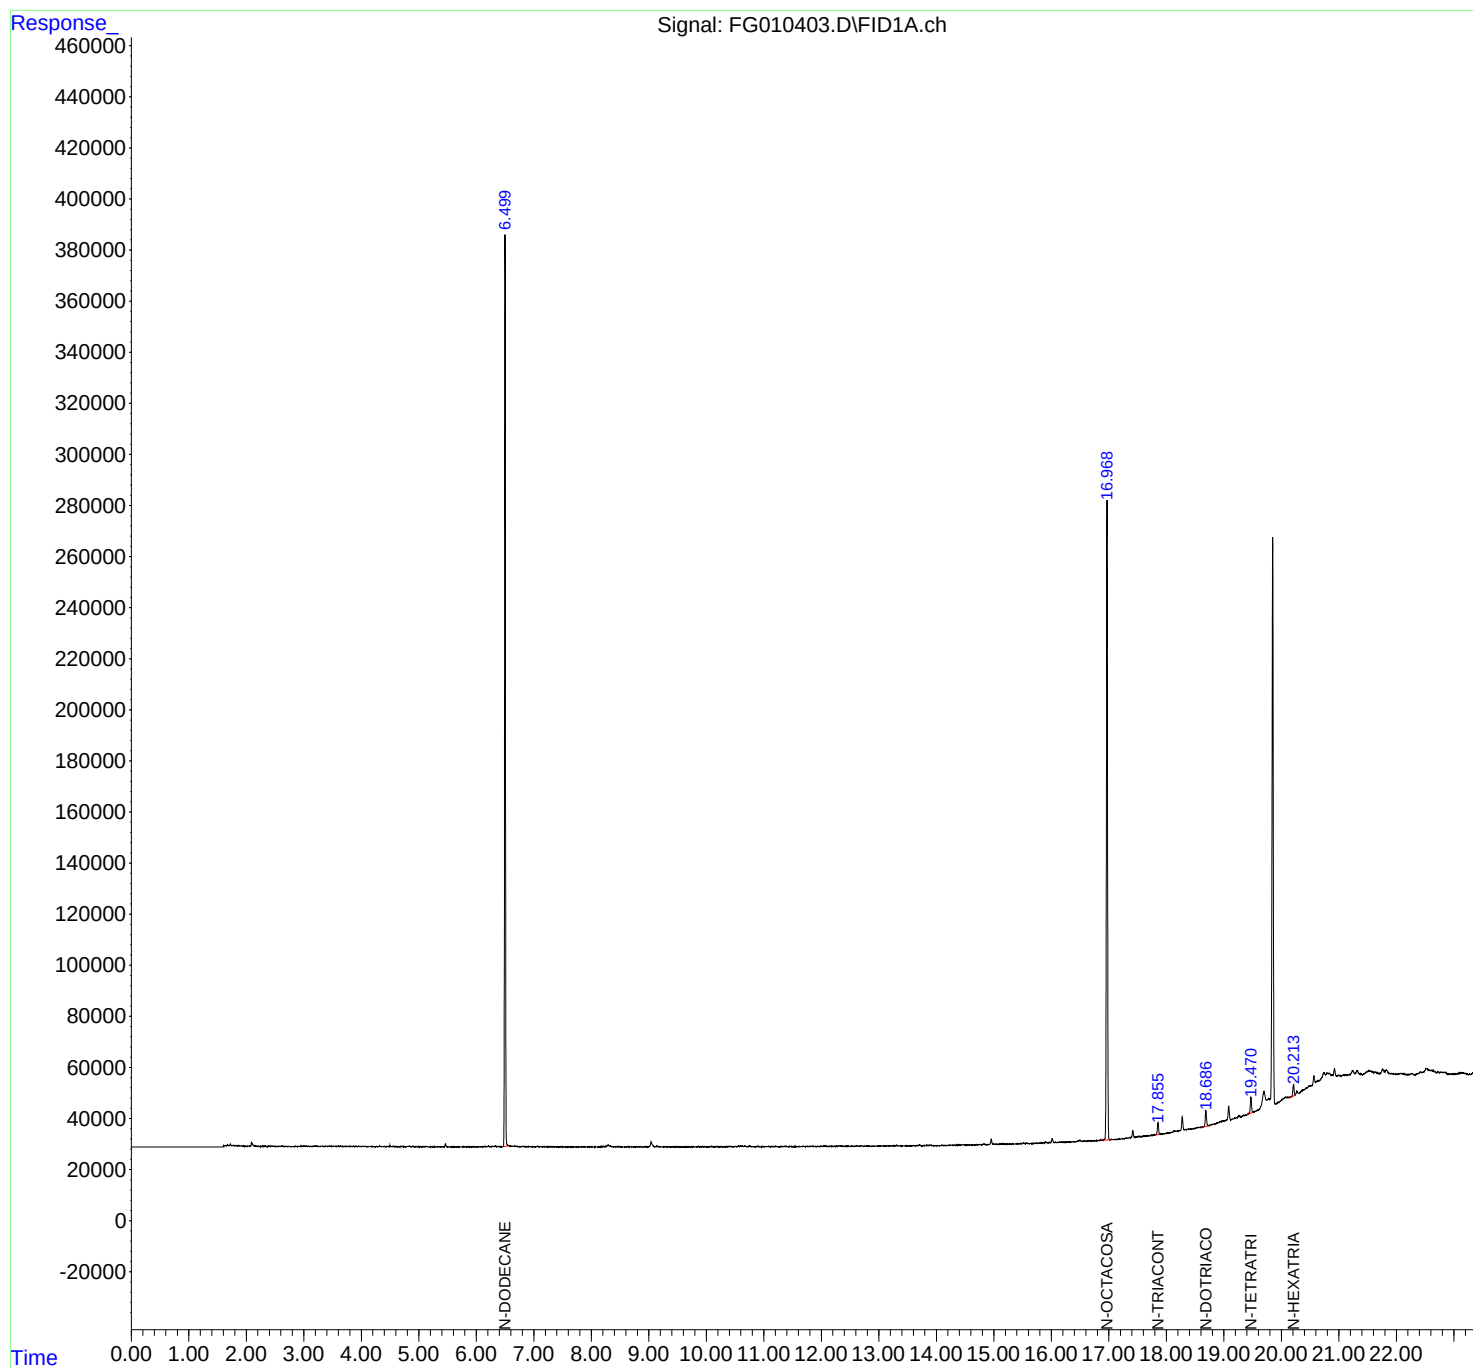


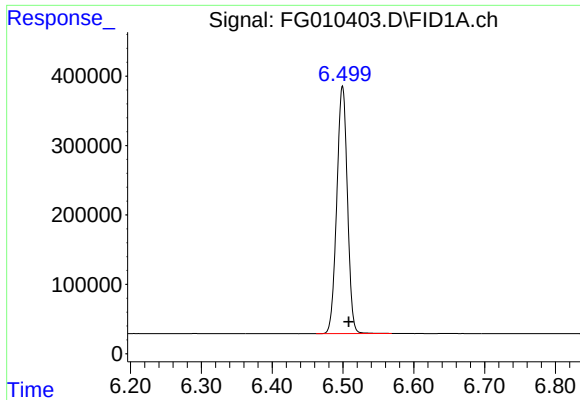

#3 N-DODECANE


R.T.: 6.499 min
Delta R.T.: -0.009 min
Response: 3719750
Conc: 27.06 ug/ml

Instrument :
FID_G
ClientSampleId :

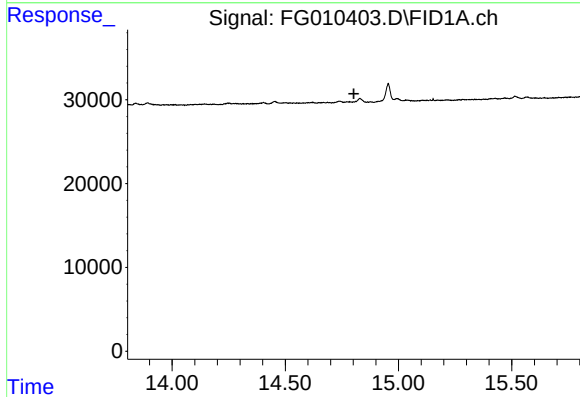


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.803 min
Response: 0
Conc: N.D.

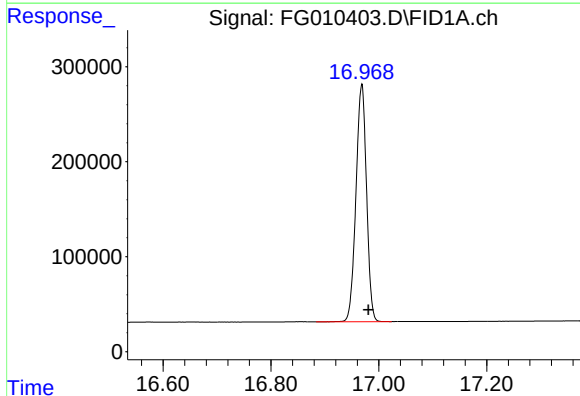


#12 N-OCTACOSANE

R.T.: 16.968 min
Delta R.T.: -0.012 min
Response: 3399034
Conc: 24.62 ug/ml

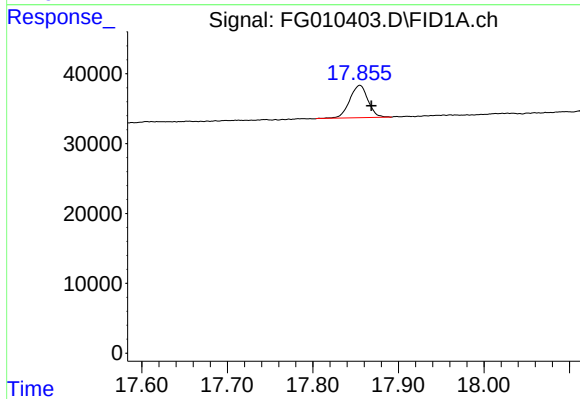

#13 N-TRIACONTANE


R.T.: 17.855 min
Delta R.T.: -0.014 min
Response: 68596
Conc: 0.51 ug/ml

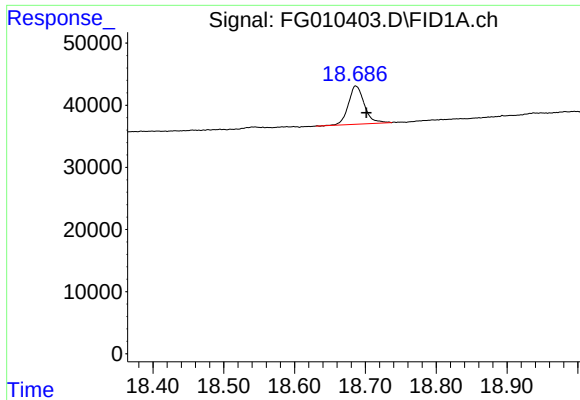

#14 N-DOTRIACONTANE


R.T.: 18.686 min
Delta R.T.: -0.015 min
Response: 96915
Conc: 0.74 ug/ml

Instrument :
FID_G
ClientSampleId :

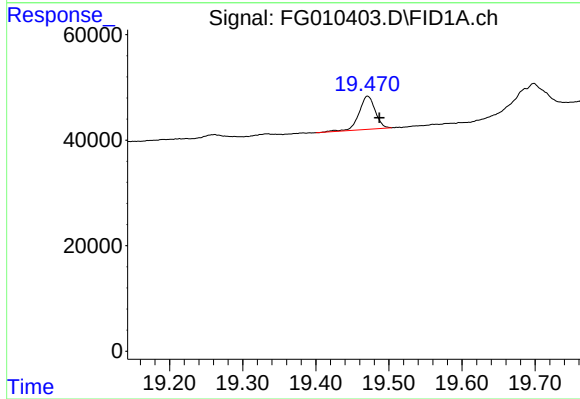

#15 N-TETRATRIACONTANE

R.T.: 19.471 min
Delta R.T.: -0.016 min
Response: 95971
Conc: 0.77 ug/ml

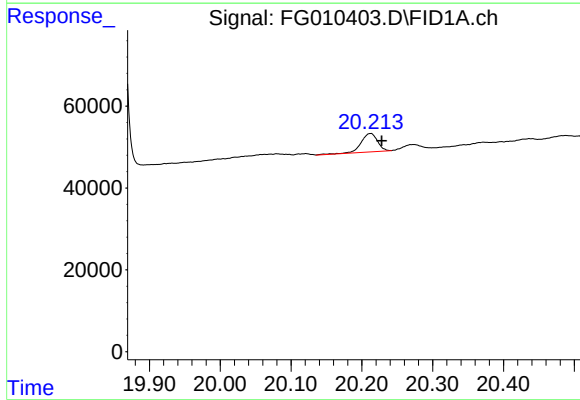

#16 N-HEXATRIACONTANE

R.T.: 20.212 min
Delta R.T.: -0.016 min
Response: 73659
Conc: 0.64 ug/ml