

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG082319\
Data File : FG005704.D
Signal(s) : FID1A.ch
Acq On : 23 Aug 2019 12:06
Operator : DD\AJ
Sample : K4462-02 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SB-46-COMP

Integration File: autoint1.e
Quant Time: Aug 24 09:10:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080819.M
Quant Title :
QLast Update : Thu Aug 08 16:03:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.749	333226	2.608 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG082319\
Data File : FG005704.D
Signal(s) : FID1A.ch
Acq On : 23 Aug 2019 12:06
Operator : DD\AJ
Sample : K4462-02 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SB-46-COMP

Integration File: autoint1.e
Quant Time: Aug 24 09:10:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG080819.M
Quant Title :
QLast Update : Thu Aug 08 16:03:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

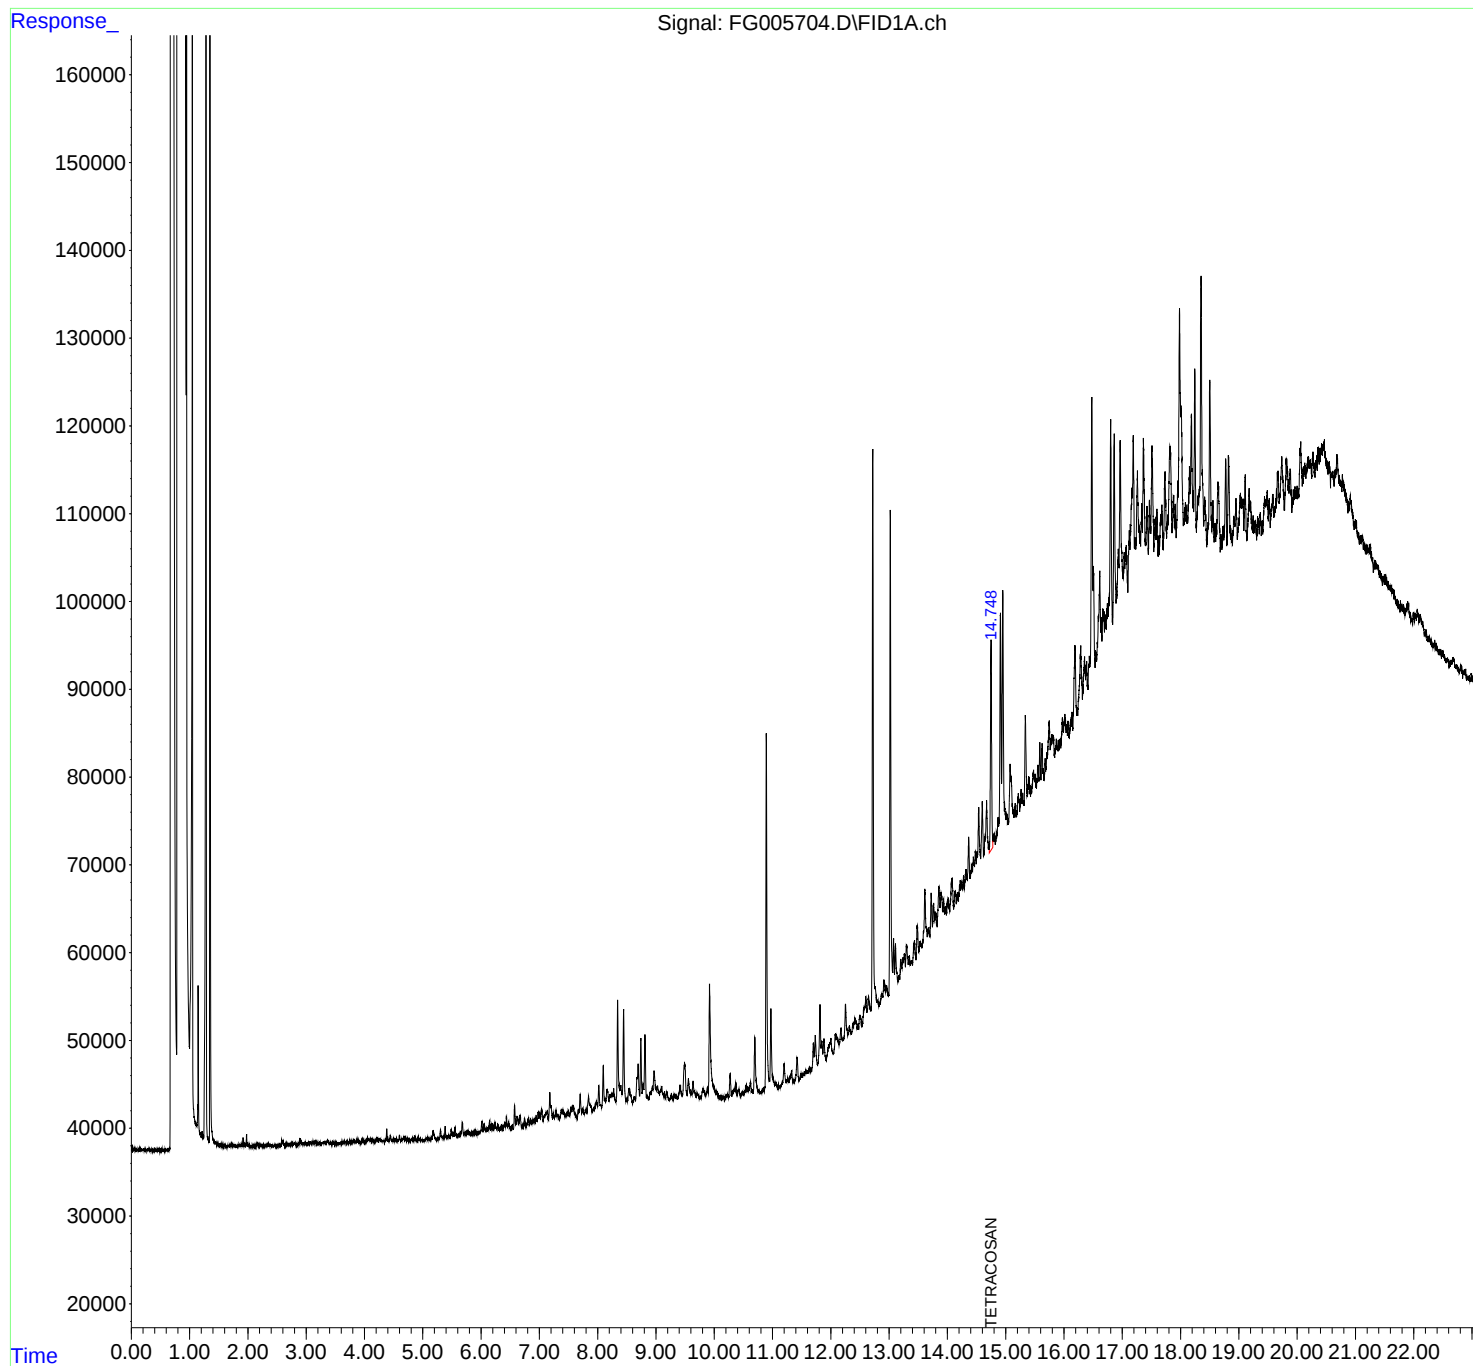

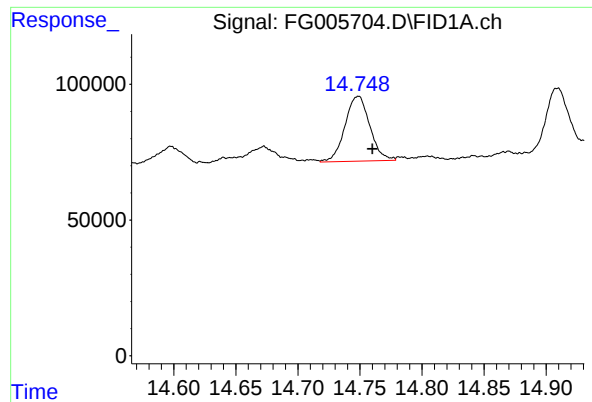

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.749 min
Delta R.T.: -0.011 min
Response: 333226
Conc: 2.61 ug/ml

Instrument :
FID_G
ClientSampleId :
SB-46-COMP